
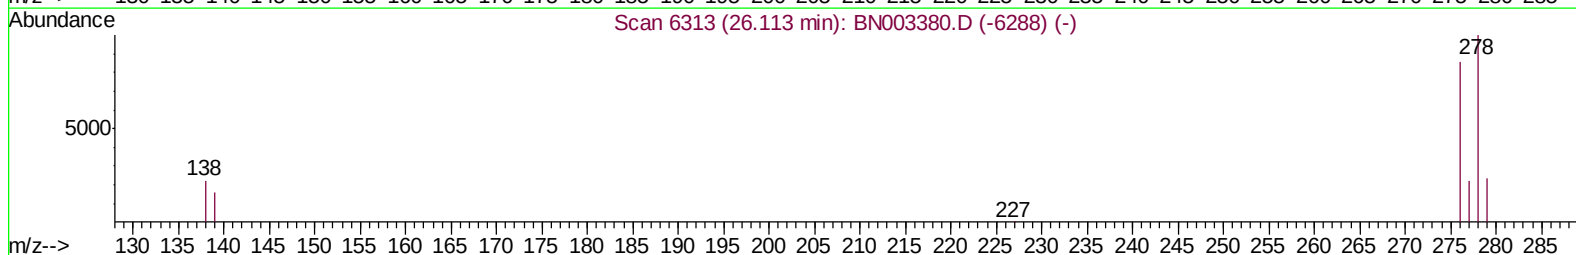
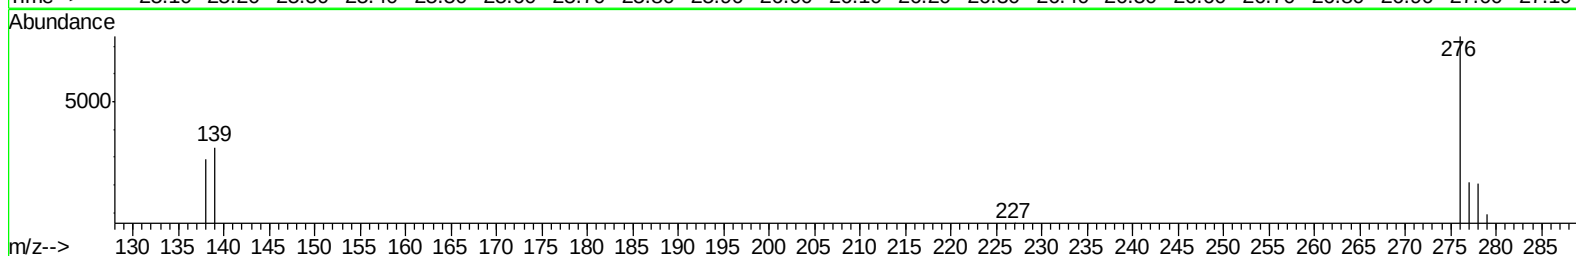


Data File : BN003393.D
Acq On : 01 Nov 2018 23:41
Operator : MJ/SJ
Sample : J5704-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Nov 02 05:58:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

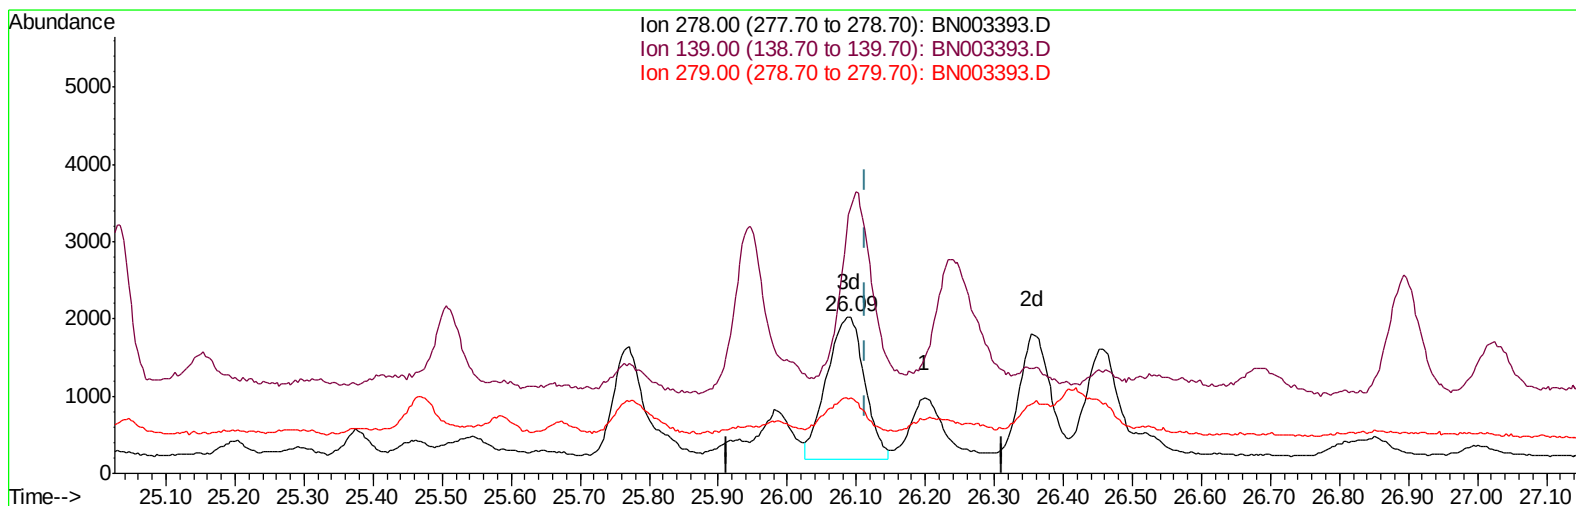

TIC: BN003393.D

(25) Dibenzo(a,h)anthracene

26.089min (-0.024) 0.04ng/ul m

response 7004

Ion	Exp%	Act%
278.00	100	100
139.00	16.40	165.38#
279.00	24.40	47.51#
0.00	0.00	0.00