
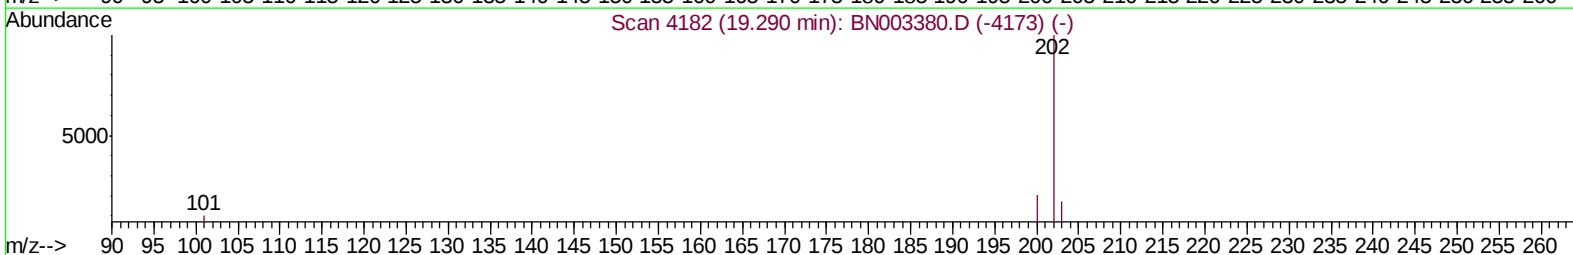
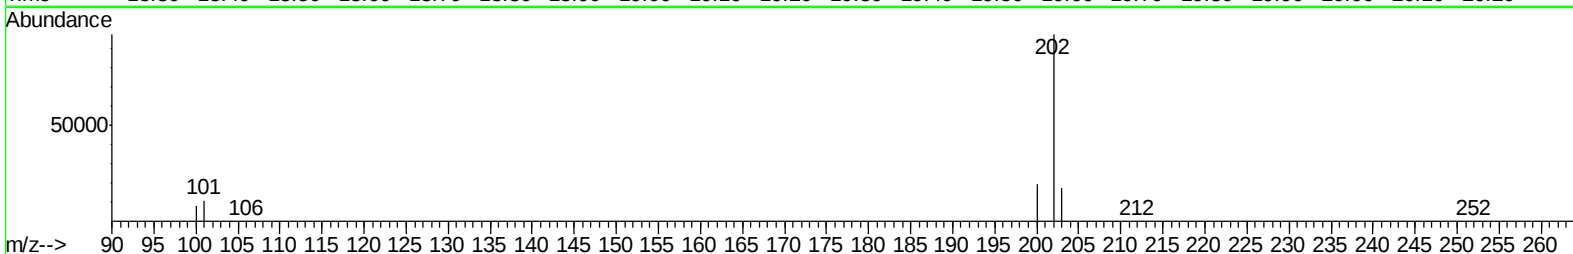


Data File : BN003394.D
Acq On : 02 Nov 2018 00:16
Operator : MJ/SJ
Sample : J5704-22
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Nov 02 06:01:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

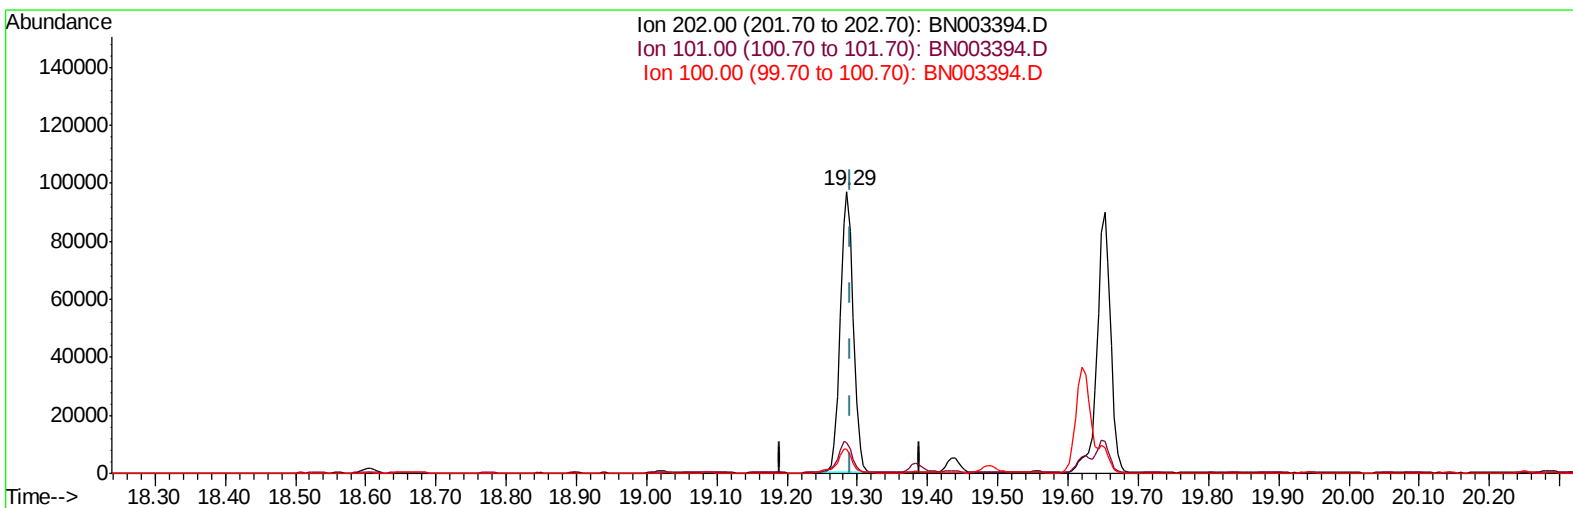

TIC: BN003394.D

(15) Fluoranthene (C)

19.285min (-0.005) 0.52ng/ul m

response 124816

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	11.12
100.00	8.00	8.45
0.00	0.00	0.00