
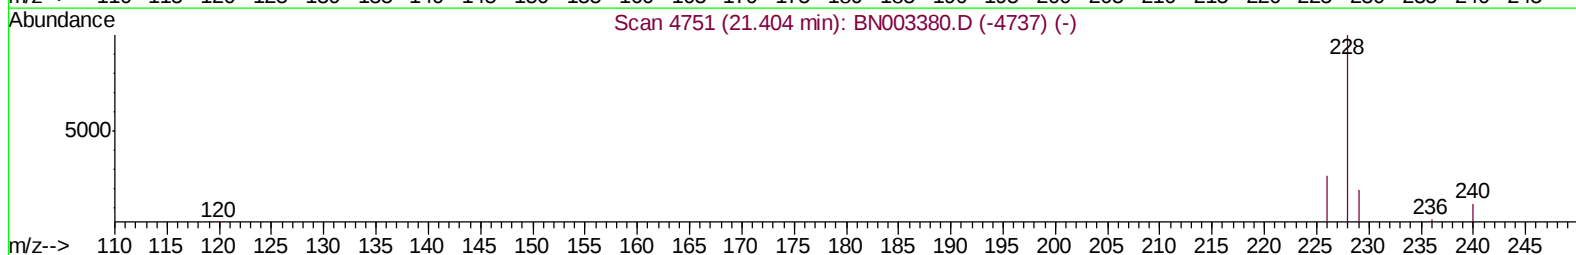
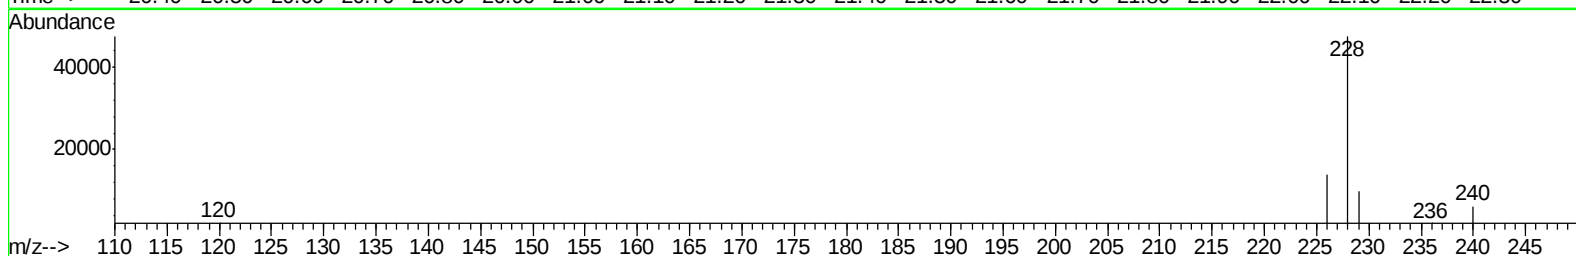


Data File : BN003394.D
Acq On : 02 Nov 2018 00:16
Operator : MJ/SJ
Sample : J5704-22
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Nov 02 06:03:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

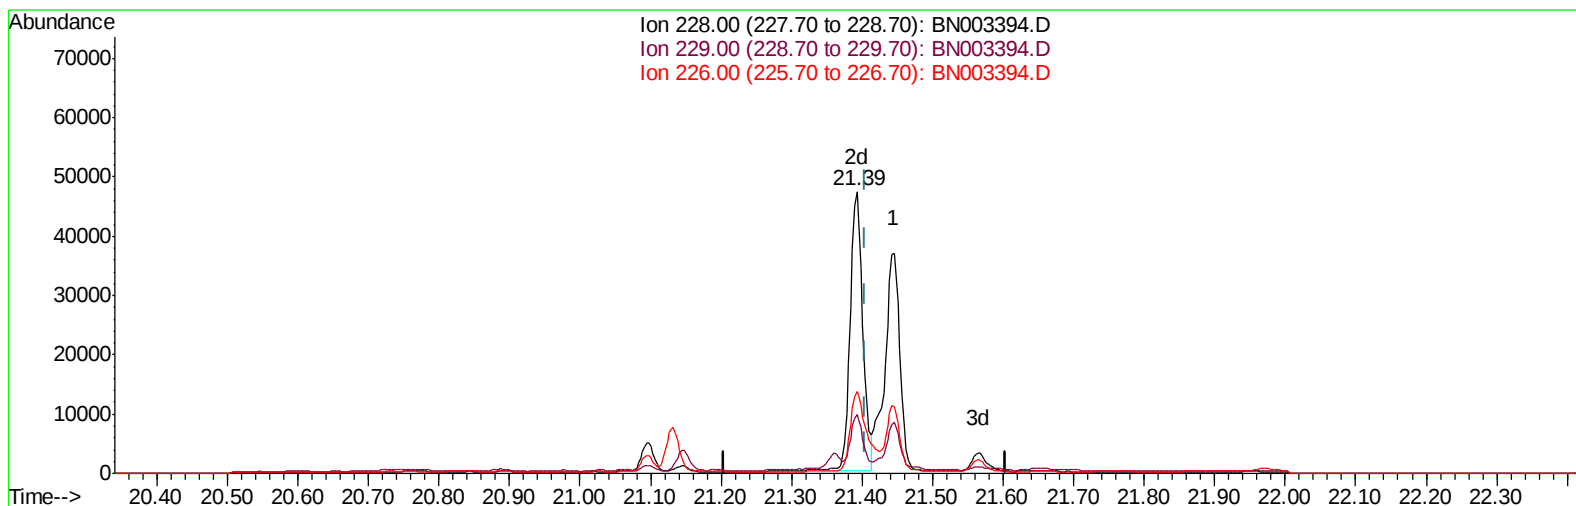

TIC: BN003394.D

(18) Benzo(a)anthracene
21.392min (-0.012) 0.32ng/ul m
response 58257

Ion	Exp%	Act%
228.00	100	100
229.00	19.40	20.94
226.00	26.90	29.25
0.00	0.00	0.00