
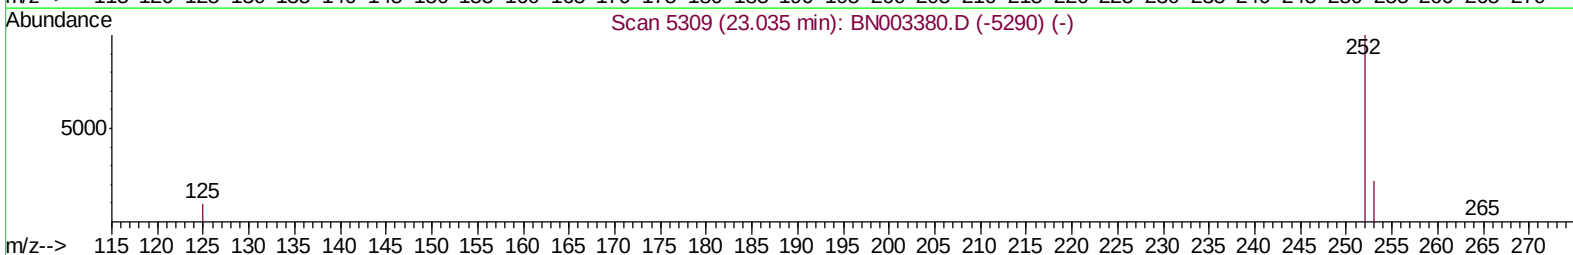
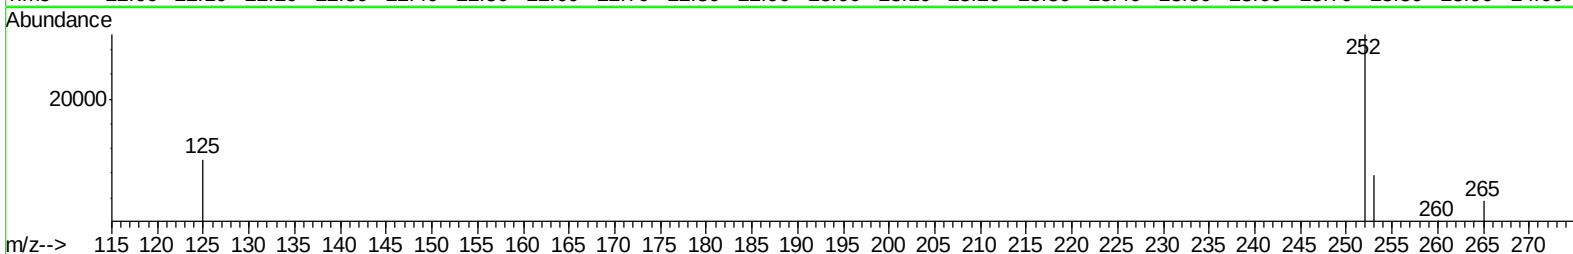


Data File : BN003394.D
Acq On : 02 Nov 2018 00:16
Operator : MJ/SJ
Sample : J5704-22
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Nov 02 06:05:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

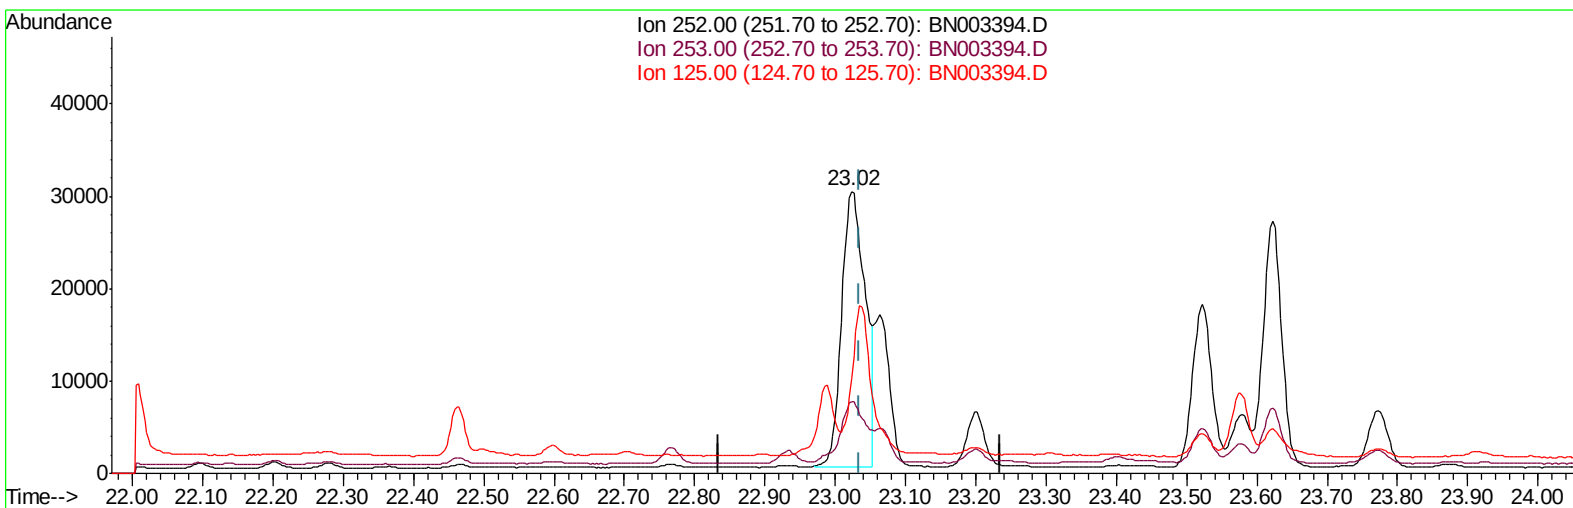

TIC: BN003394.D

(21) Benzo(b)fluoranthene

23.023min (-0.012) 0.35ng/ul m

response 69443

Ion	Exp%	Act%
252.00	100	100
253.00	22.80	25.43
125.00	10.90	33.67#
0.00	0.00	0.00