
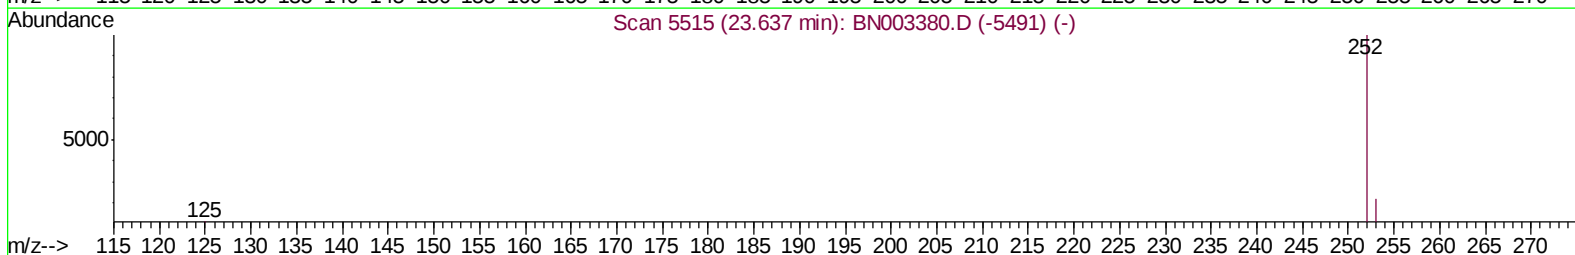
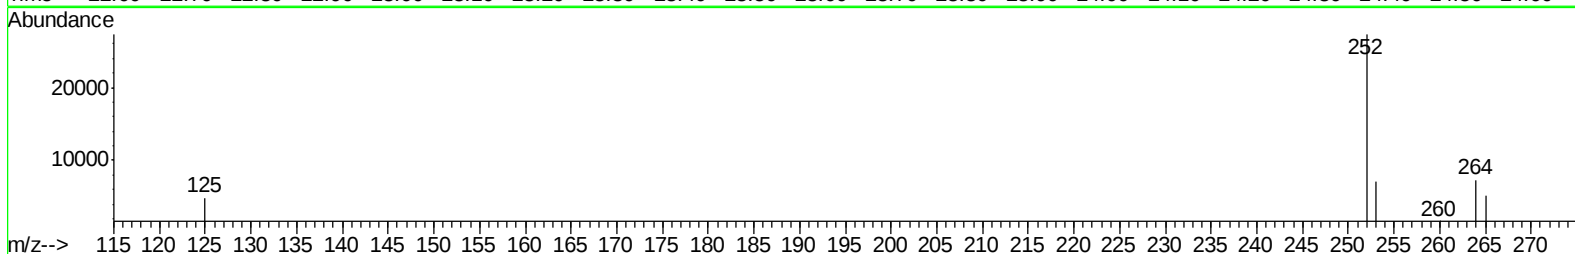


Data File : BN003394.D
Acq On : 02 Nov 2018 00:16
Operator : MJ/SJ
Sample : J5704-22
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Nov 02 06:05:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 04:49:17 2018
Response via : Initial Calibration

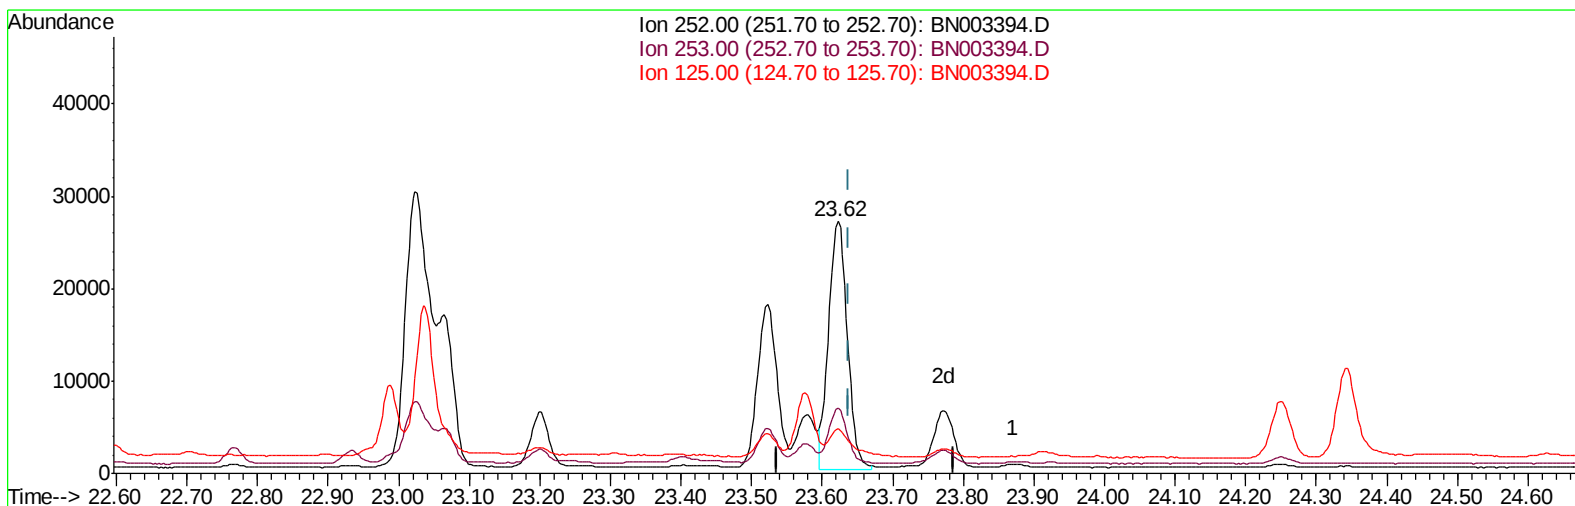

TIC: BN003394.D

(23) Benzo(a)pyrene (C)

23.623min (-0.015) 0.29ng/ul m

response 48964

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	25.68
125.00	12.40	17.58#
0.00	0.00	0.00