


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110122\
 Data File : BN022443.D
 Acq On : 01 Nov 2022 19:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 02 05:31:40 2022

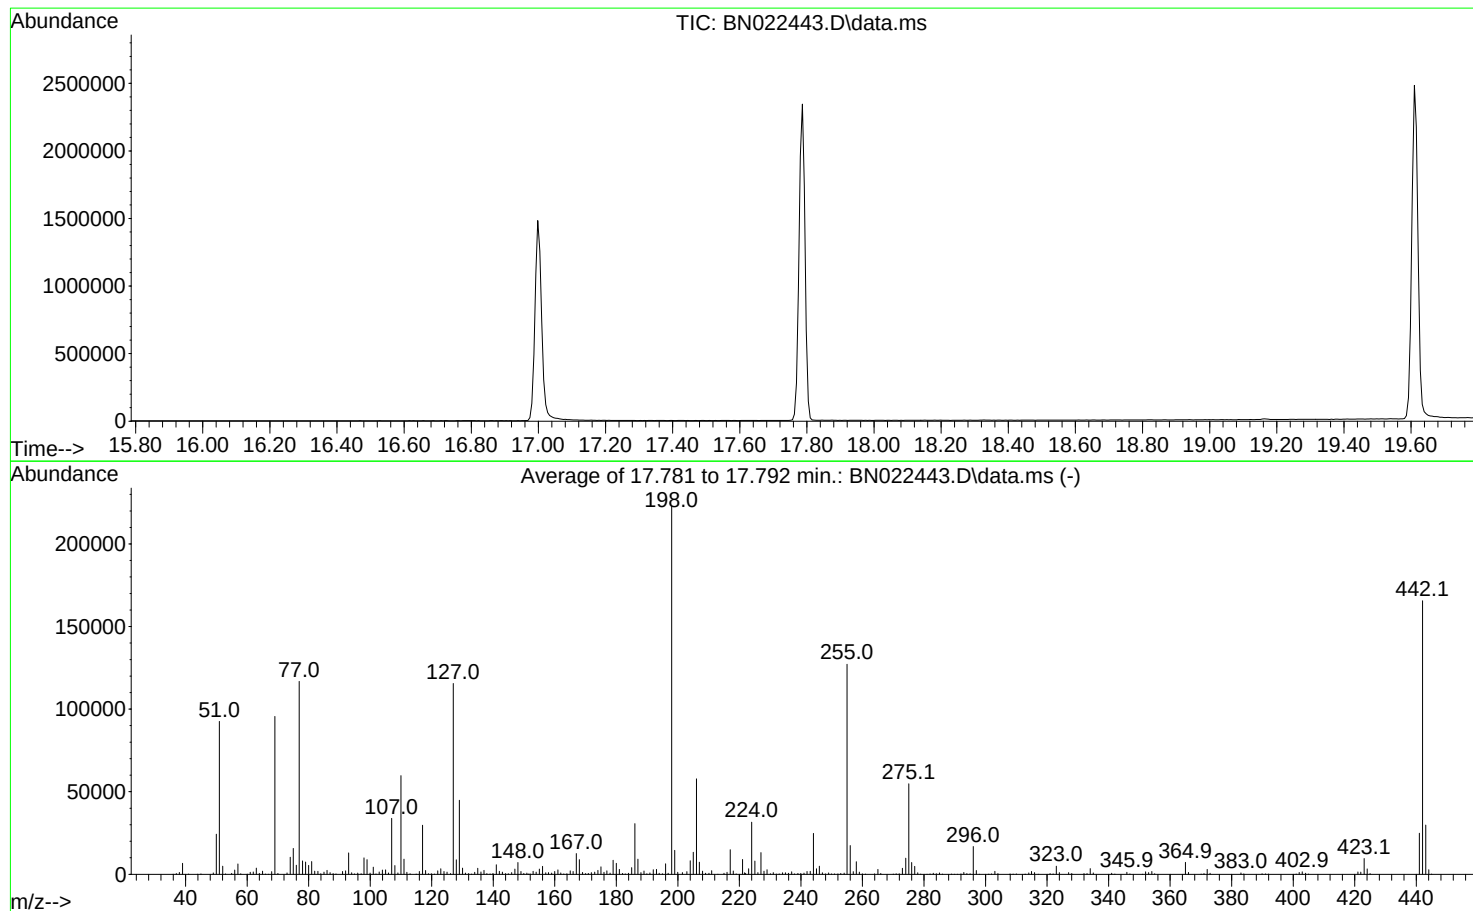




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	92603	PASS
68	69	0.00	2	1.7	1655	PASS
69	198	0.00	100	42.9	95597	PASS
70	69	0.00	2	0.6	546	PASS
127	198	10	80	51.9	115491	PASS
197	198	0.00	2	0.3	616	PASS
198	198	100	100	100.0	222720	PASS
199	198	5	9	6.5	14440	PASS
275	198	10	60	24.6	54776	PASS
365	198	1	100	3.2	7179	PASS
441	198	0.01	100	11.1	24808	PASS
442	442	50	100	100.0	165581	PASS
443	442	15	24	18.0	29837	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110122\
Data File : BN022443.D
Acq On : 01 Nov 2022 19:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 02 06:46:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 06:46:31 2022
Response via : Initial Calibration

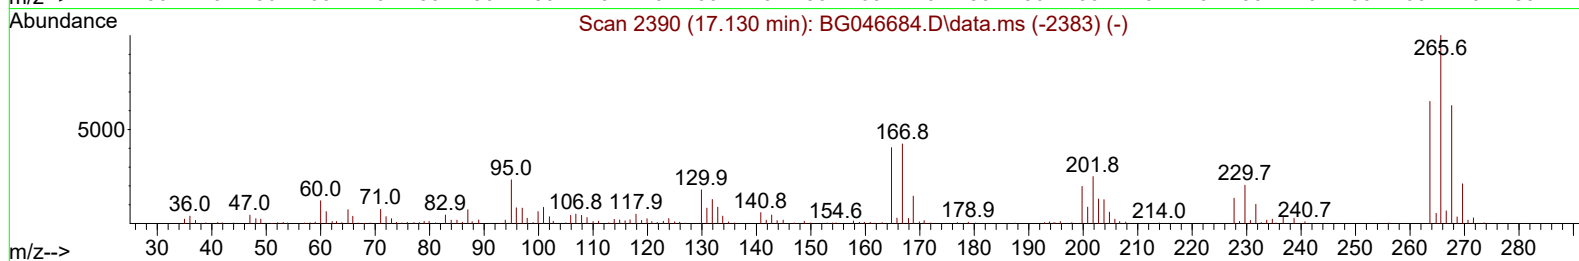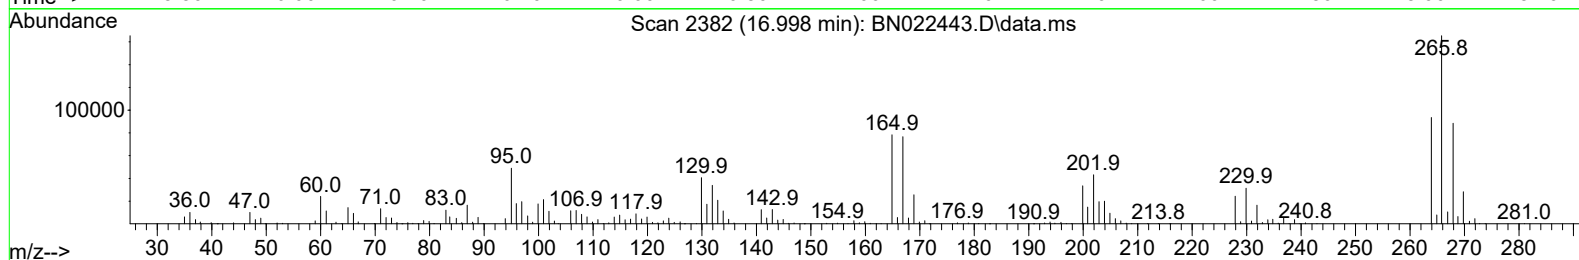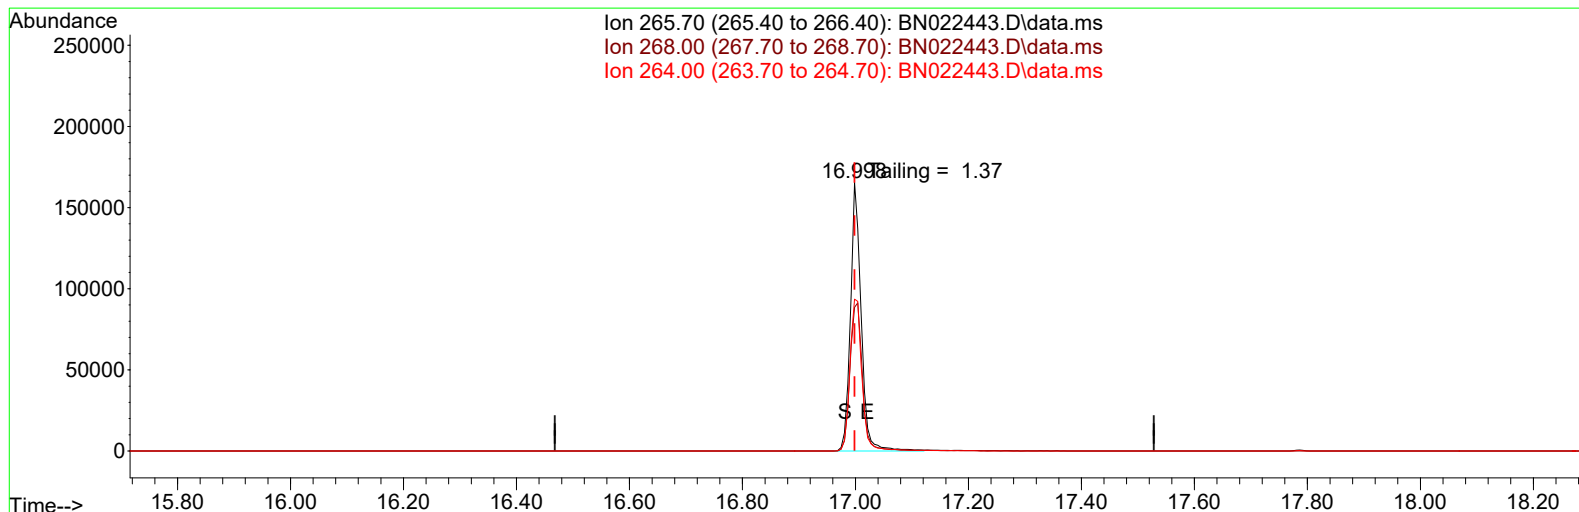

TIC: BN022443.D\data.ms

(70) Pentachlorophenol (C)

16.998min (0.000) 18796.44 ng




response 220232

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	53.52
264.00	61.60	56.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110122\
Data File : BN022443.D
Acq On : 01 Nov 2022 19:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 02 06:46:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 06:46:31 2022
Response via : Initial Calibration

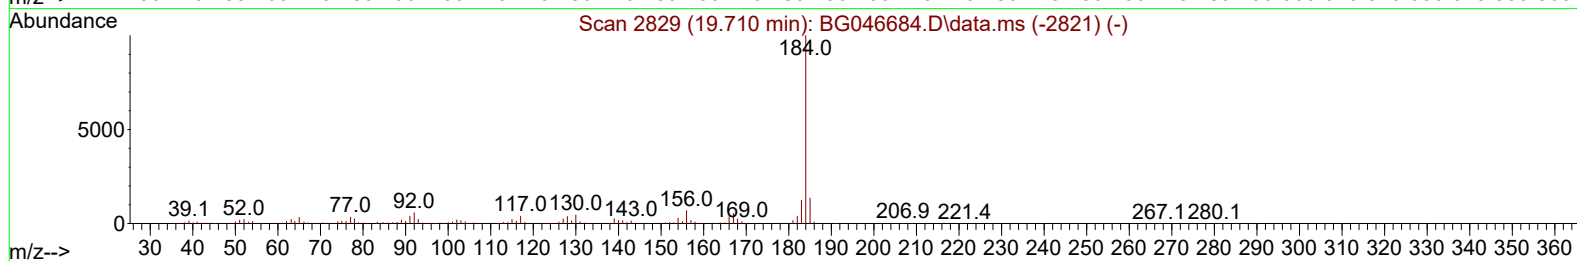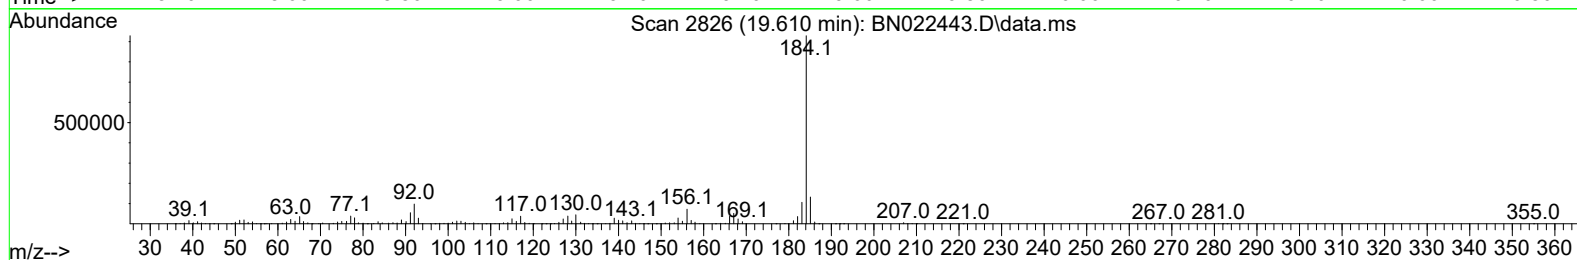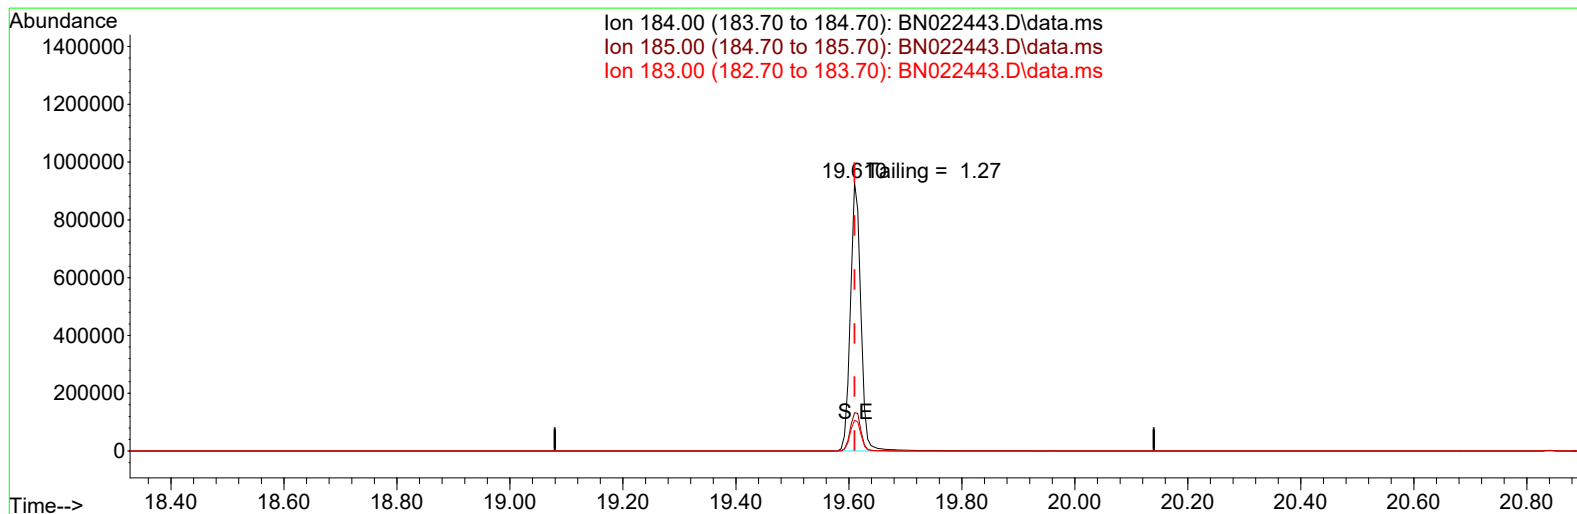

TIC: BN022443.D\data.ms

(77) Benzidine

19.610min (0.000) 0.00 ng

response 1203174

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.25
183.00	13.20	11.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/1/2022	BNA_N	<u>BN022443.D</u>
Compound Name	Response	Retention Time
DDT	584312	20.839
DDD	13252	20.404
DDE	591	19.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13843	598155	2.31

Instrument :
BNA_N
ClientSampleId :
DFTPP