
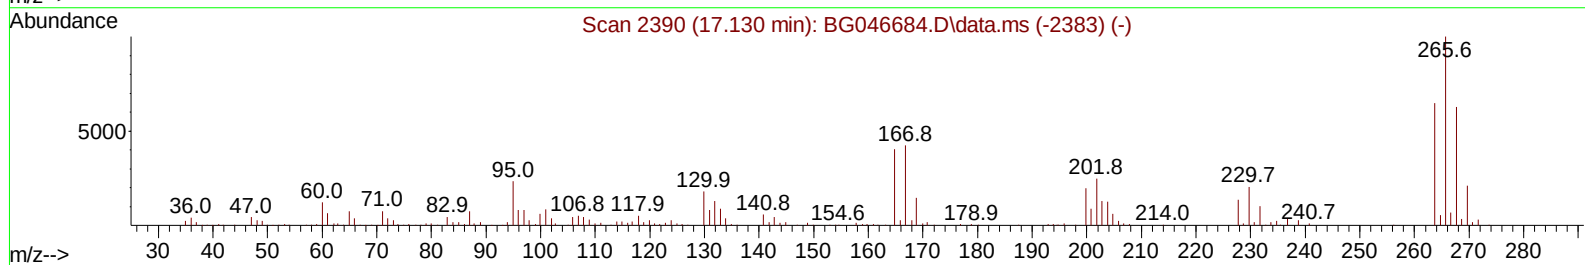
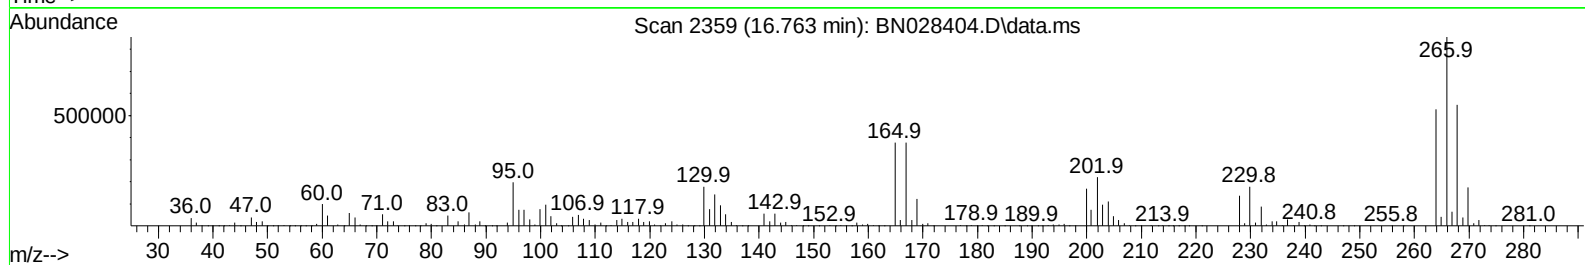


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110123\
Data File : BN028404.D
Acq On : 01 Nov 2023 17:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 08:07:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 02 08:07:37 2023
Response via : Initial Calibration

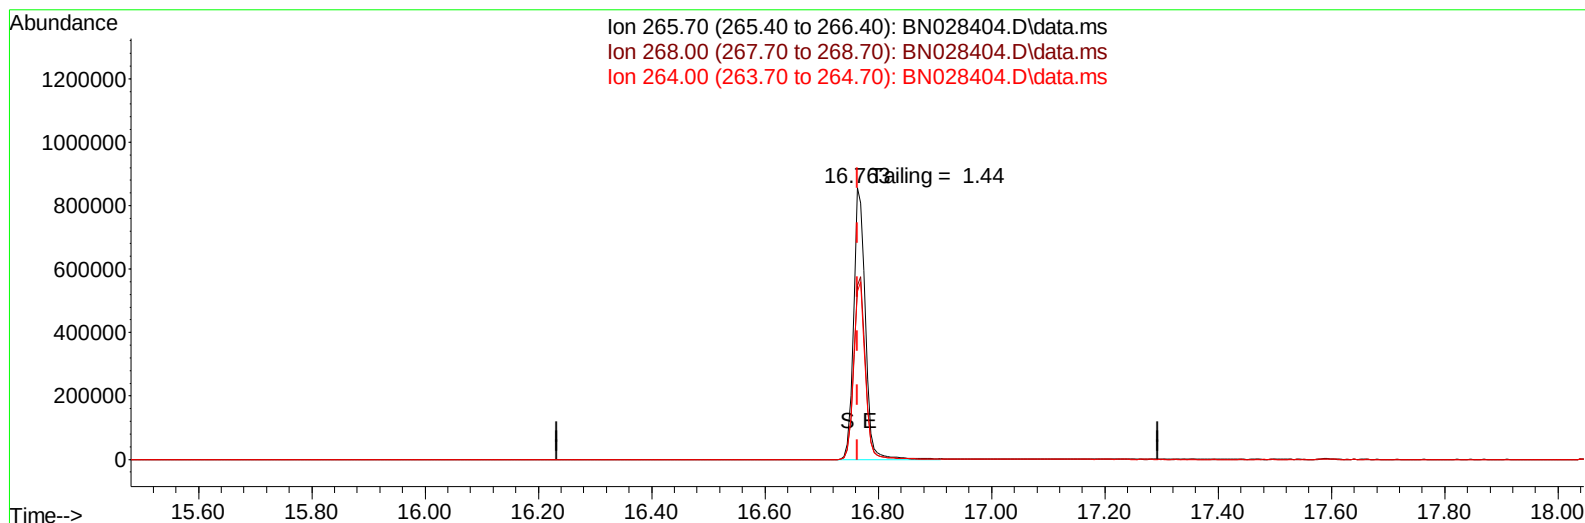

TIC: BN028404.D\data.ms

(70) Pentachlorophenol (C)




16.763min (0.000) 26763.25 ng

response 1242545

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.00
264.00	61.60	61.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110123\
 Data File : BN028404.D
 Acq On : 01 Nov 2023 17:34
 Operator : MA/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 08:07:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 02 08:07:37 2023
 Response via : Initial Calibration

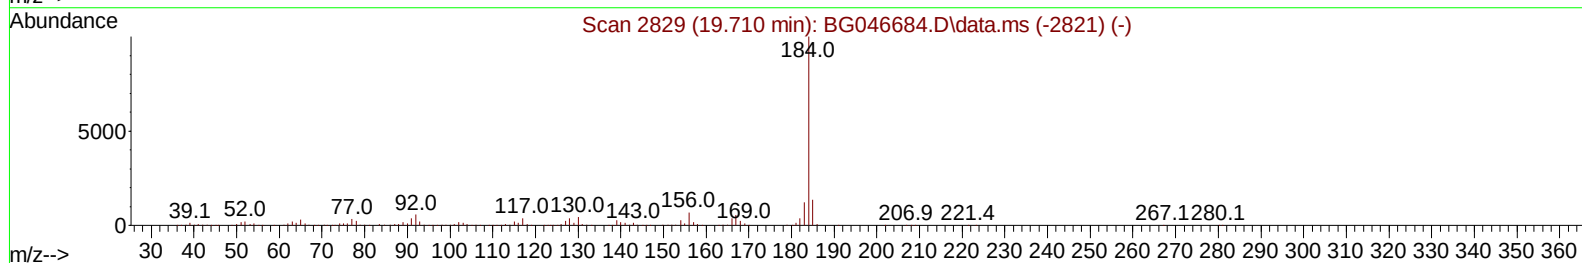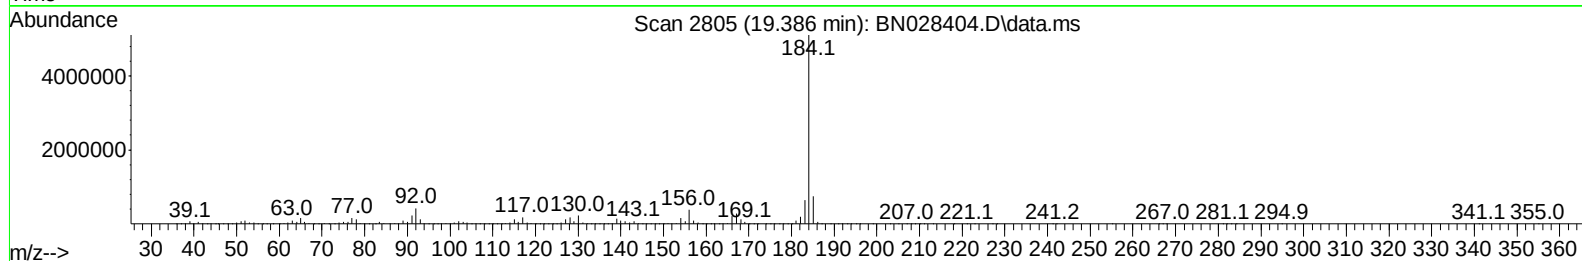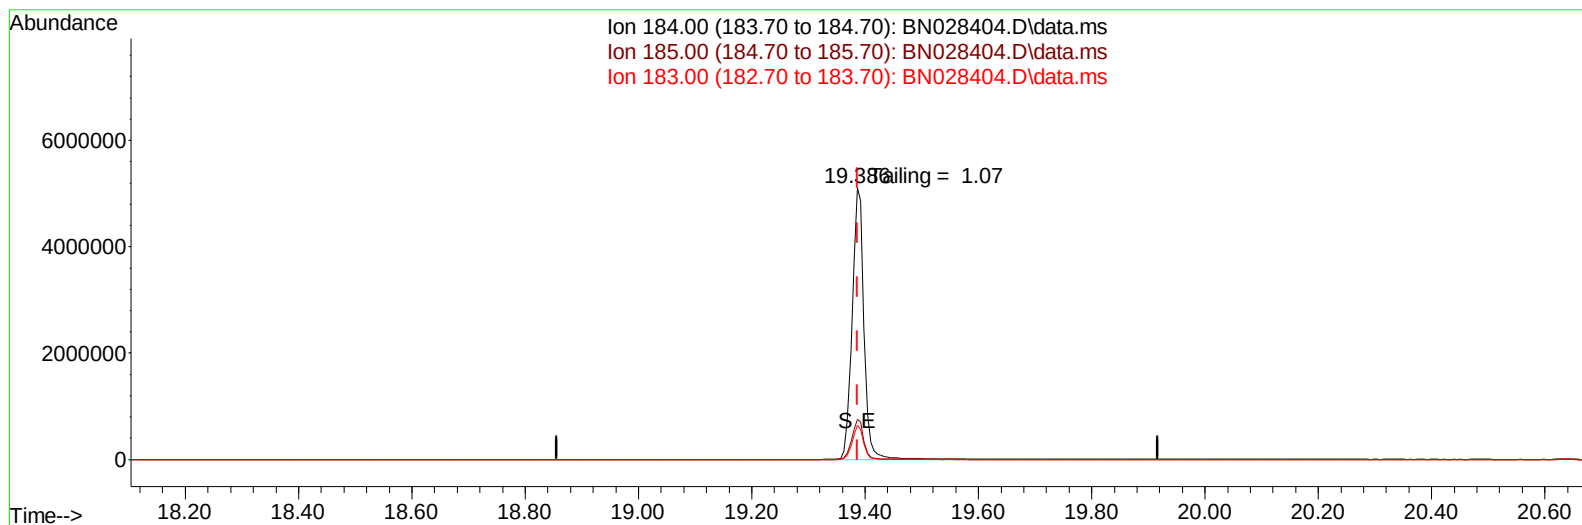

TIC: BN028404.D\data.ms

(77) Benzidine**19.386min (0.000) 1985940.18 ng****response 7468516**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.73
183.00	13.20	12.62
0.00	0.00	0.00