
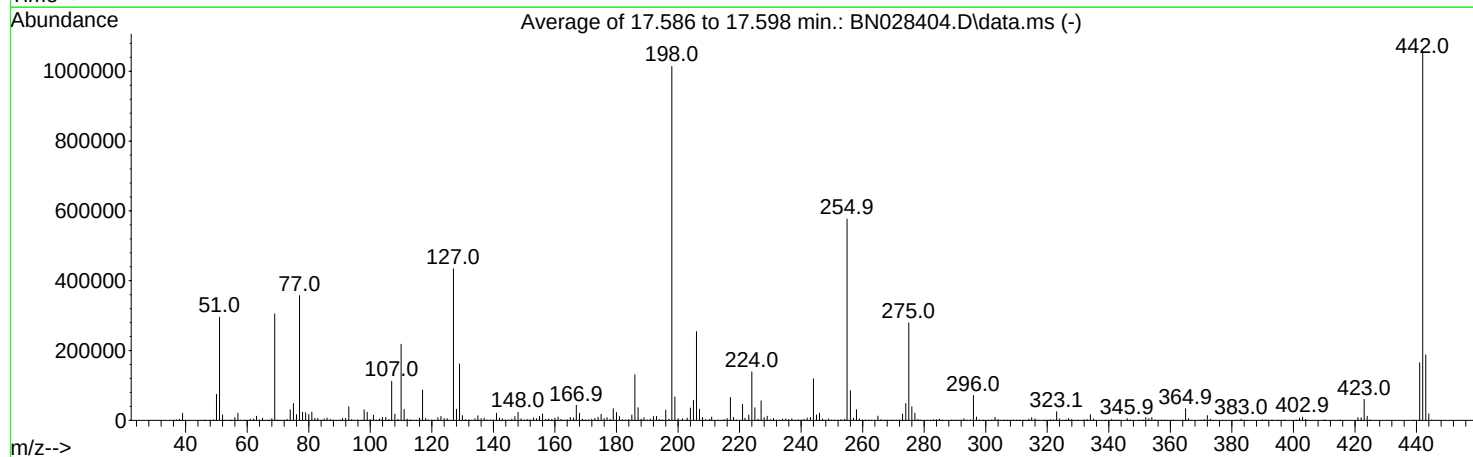


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110123\
Data File : BN028404.D
Acq On : 01 Nov 2023 17:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 02 06:26:50 2023

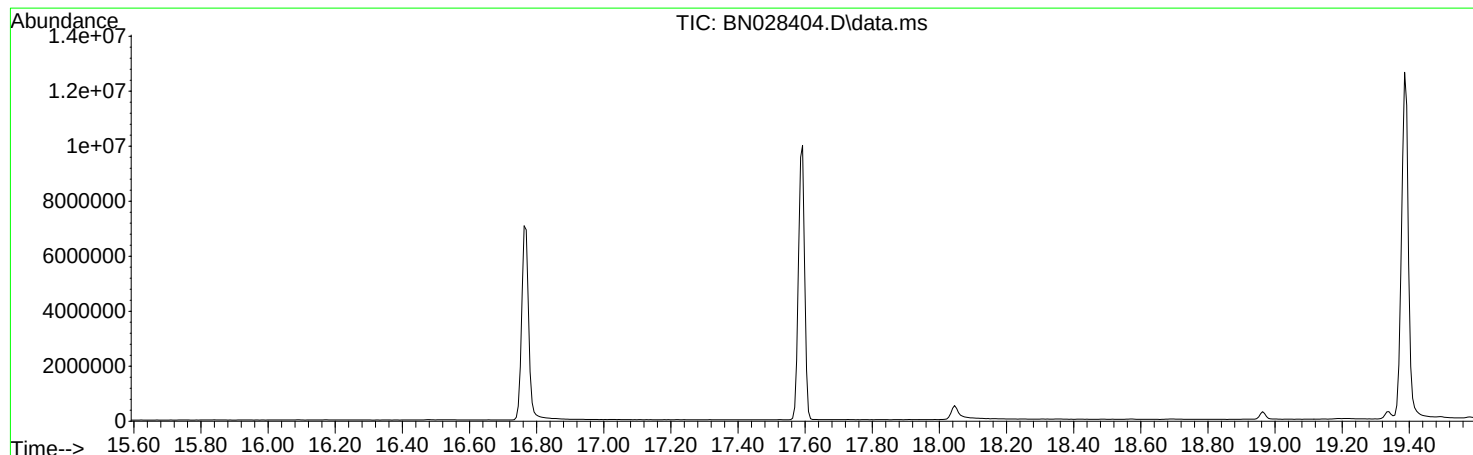




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	295697	PASS
68	69	0.00	2	1.6	5001	PASS
69	198	0.00	100	30.1	305163	PASS
70	69	0.00	2	0.5	1393	PASS
127	198	10	80	42.8	434069	PASS
197	198	0.00	2	0.3	3519	PASS
198	198	100	100	100.0	1014037	PASS
199	198	5	9	6.6	66947	PASS
275	198	10	60	27.5	279360	PASS
365	198	1	100	3.3	33501	PASS
441	198	0.01	100	16.3	164885	PASS
442	442	50	100	100.0	1053824	PASS
443	442	15	24	17.8	187349	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110123\
Data File : BN028404.D
Acq On : 01 Nov 2023 17:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 02 08:07:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 02 08:07:37 2023
Response via : Initial Calibration

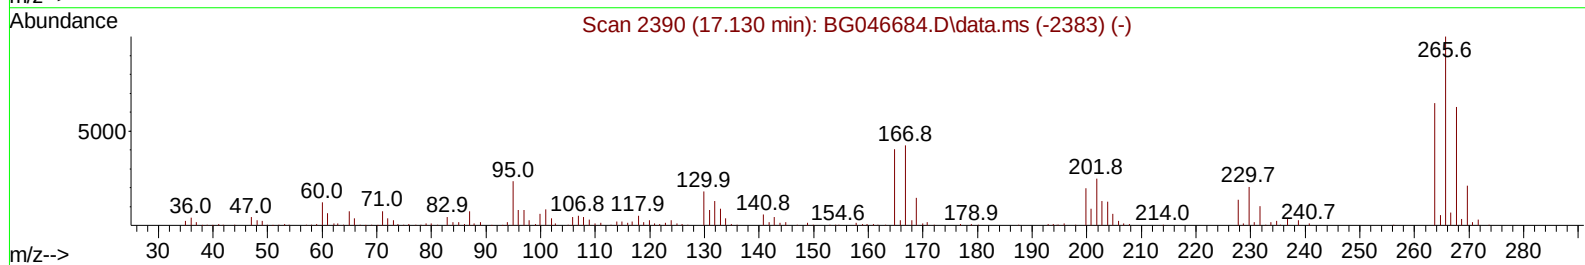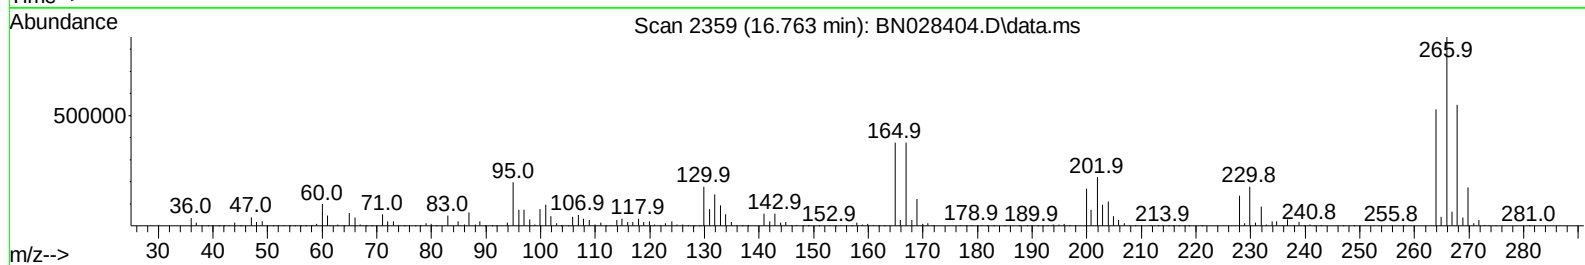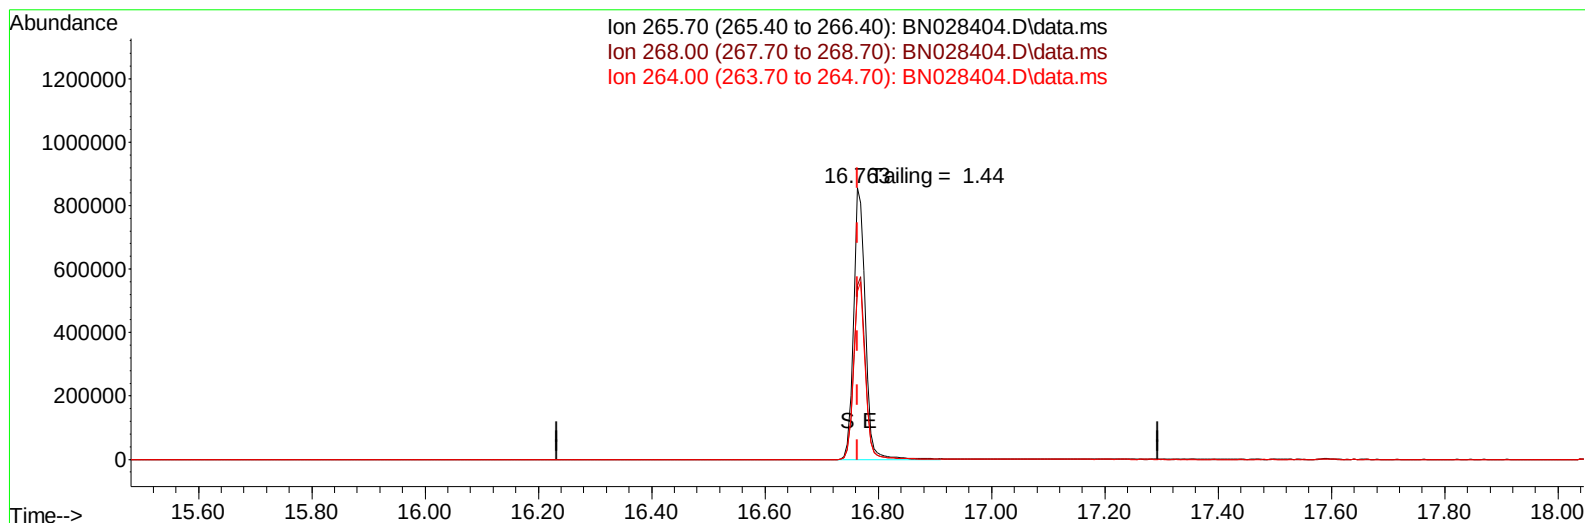

TIC: BN028404.D\data.ms

(70) Pentachlorophenol (C)

16.763min (0.000) 26763.25 ng




response 1242545

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.00
264.00	61.60	61.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110123\
Data File : BN028404.D
Acq On : 01 Nov 2023 17:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 02 08:07:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 02 08:07:37 2023
Response via : Initial Calibration

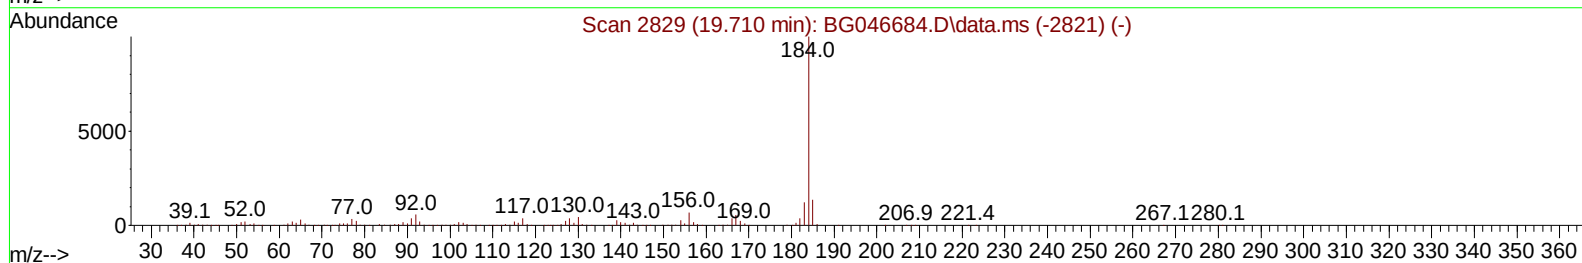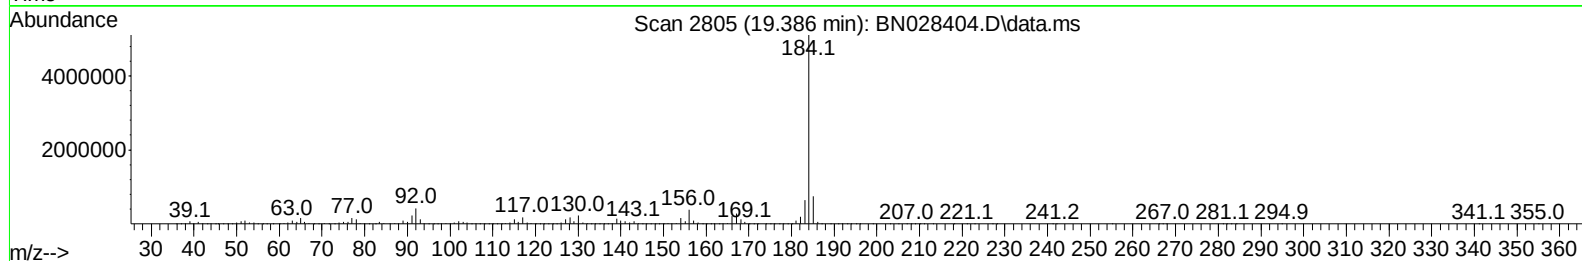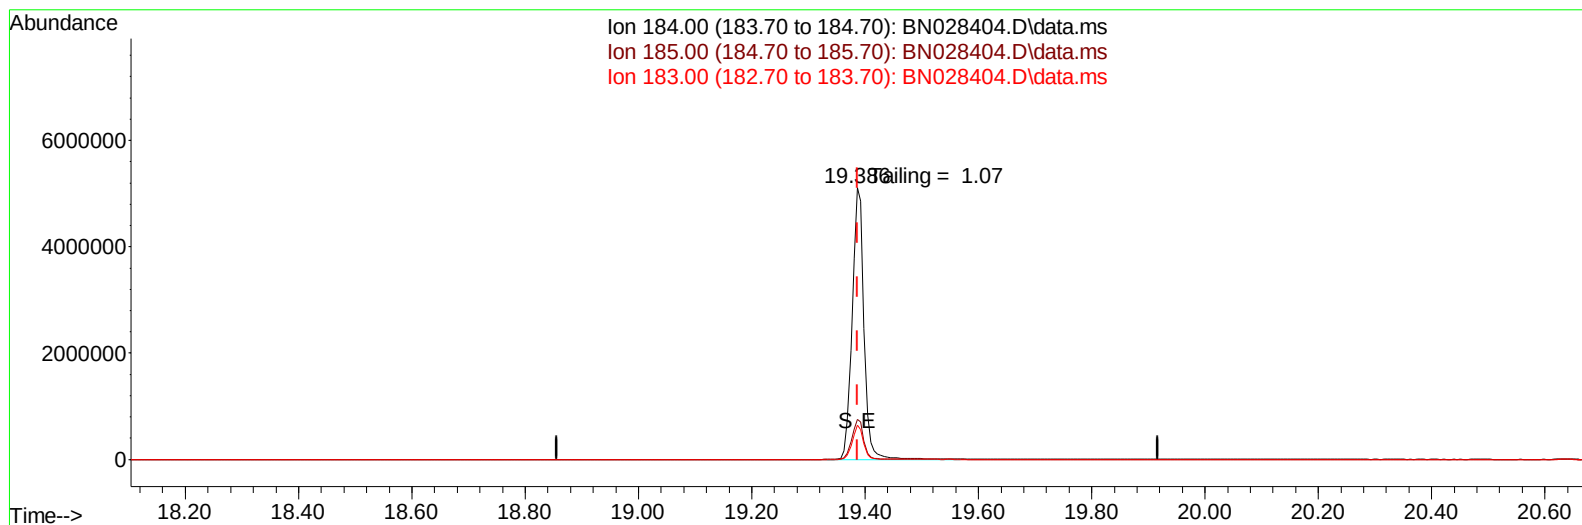

TIC: BN028404.D\data.ms

(77) Benzidine

19.386min (0.000) 1985940.18 ng

response 7468516

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.73
183.00	13.20	12.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/1/2023	BNA_N	<u>BN028404.D</u>
Compound Name	Response	Retention Time
DDT	3289474	20.639
DDD	51545	20.245
DDE	3821	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
55366	3344840	1.66

Instrument :
BNA_N
ClientSampleId :
DFTPP