

Data File : BN003406.D
Acq On : 02 Nov 2018 16:54
Operator : MJ/SJ
Sample : PB114248BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK58

Quant Time: Nov 02 23:51:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 23:49:03 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	10509	0.40	ng/ul	0.00
2) Naphthalene-d8	10.65	136	43433	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.49	164	25508	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.33	188	3193698	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.41
20) Perylene-d12	23.73	264	40426	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.24	152	20389	0.29	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.49	166	5714	0.049	ng/ul#	12
23) Benzo(a)pyrene	23.58	252	8967	0.062	ng/ul#	16


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003406.D
Acq On : 02 Nov 2018 16:54
Operator : MJ/SJ
Sample : PB114248BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK58

Quant Time: Nov 02 23:51:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 02 23:49:03 2018
Response via : Initial Calibration

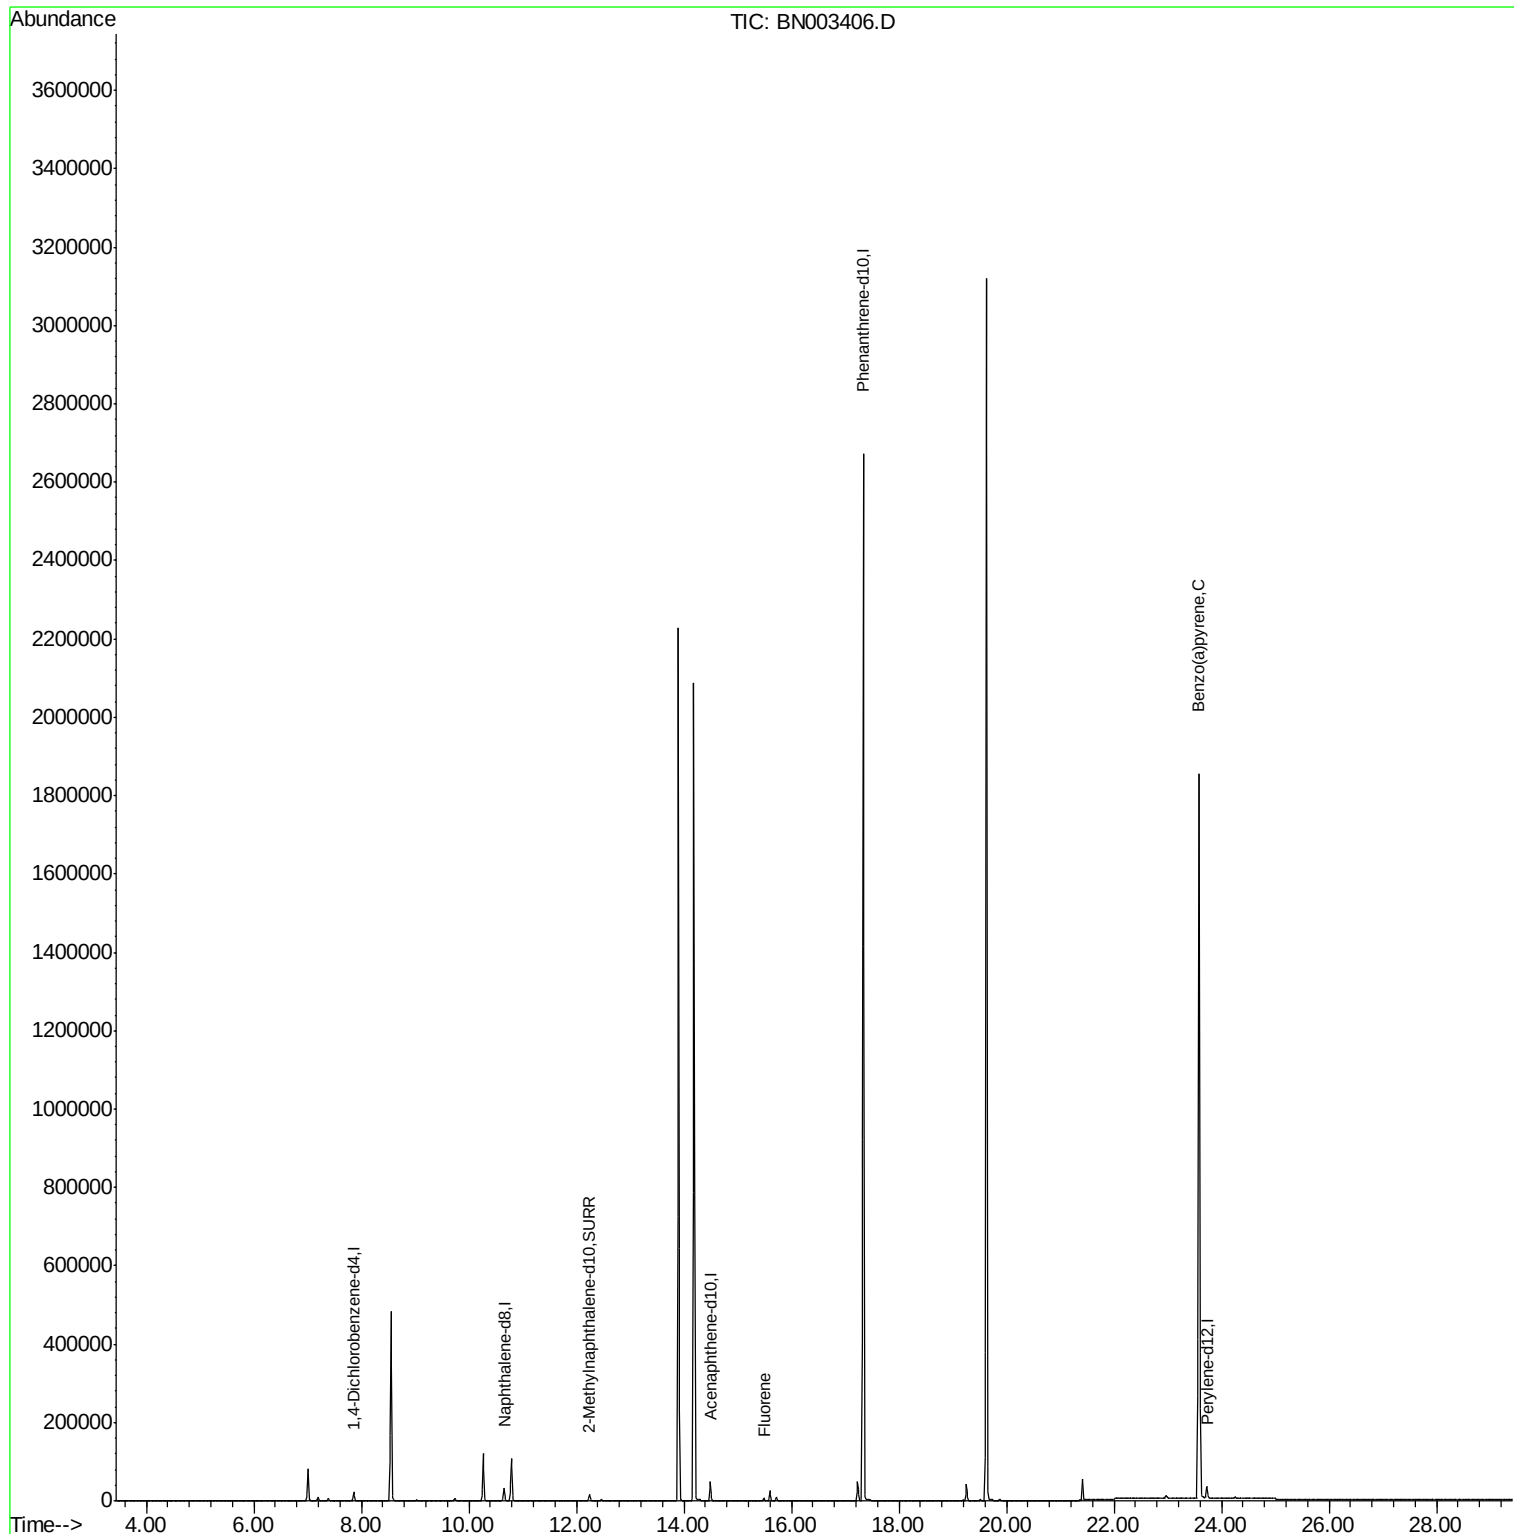

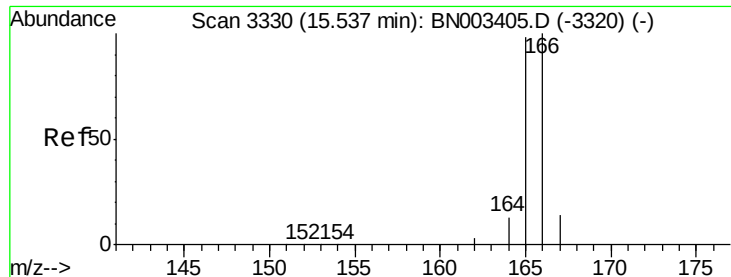

#9

Fluorene

Concen: 0.049 ng/ul

RT: 15.49 min Scan# 3319

Delta R.T. -0.05 min

Lab File: BN003406.D

Acq: 02 Nov 2018 16:54

Instrument :

BNA_N

ClientSampleId :

SBLK58


Tgt Ion:166 Resp: 5714

Ion Ratio Lower Upper

166 100

165 6.2 78.3 117.5#




167 34.9 10.8 16.2#

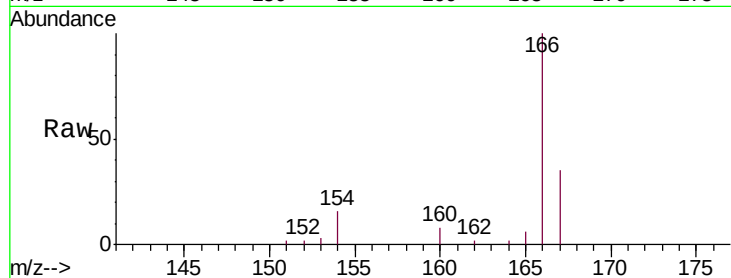

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

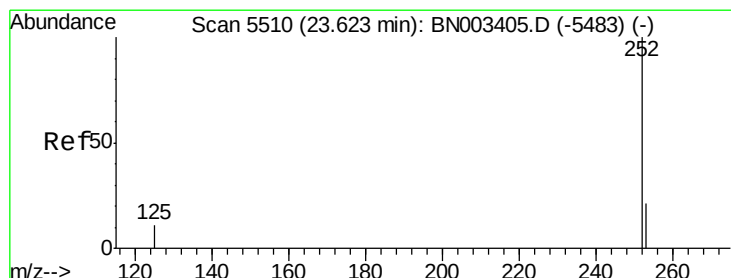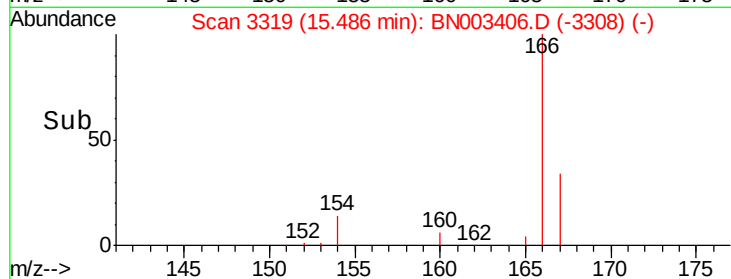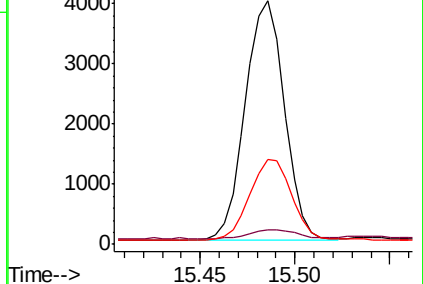

#23

Benzo(a)pyrene

Concen: 0.062 ng/ul

RT: 23.58 min Scan# 5495

Delta R.T. -0.04 min

Lab File: BN003406.D

Acq: 02 Nov 2018 16:54


Tgt Ion:252 Resp: 8967

Ion Ratio Lower Upper

252 100

253 43.7 18.5 27.7#

125 75.5 9.9 14.9#

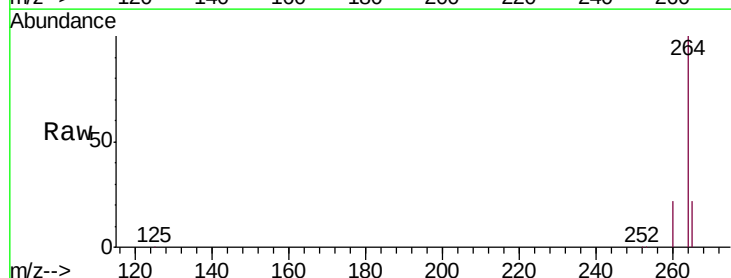

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

