
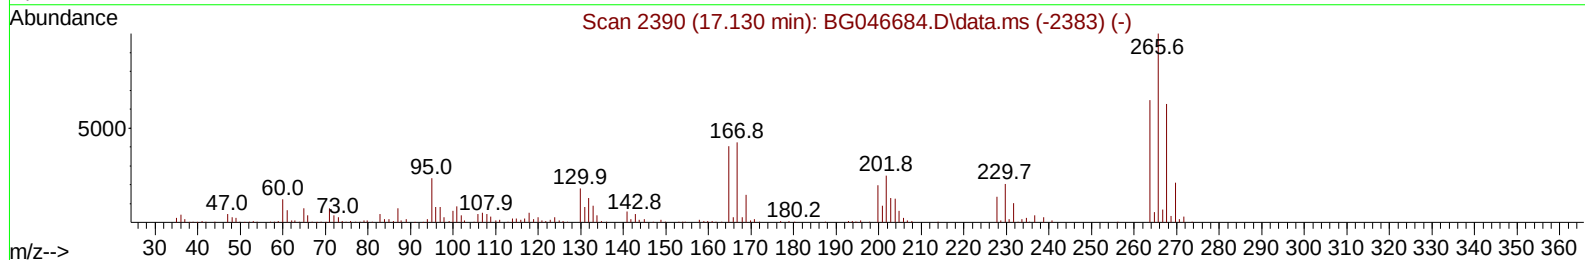
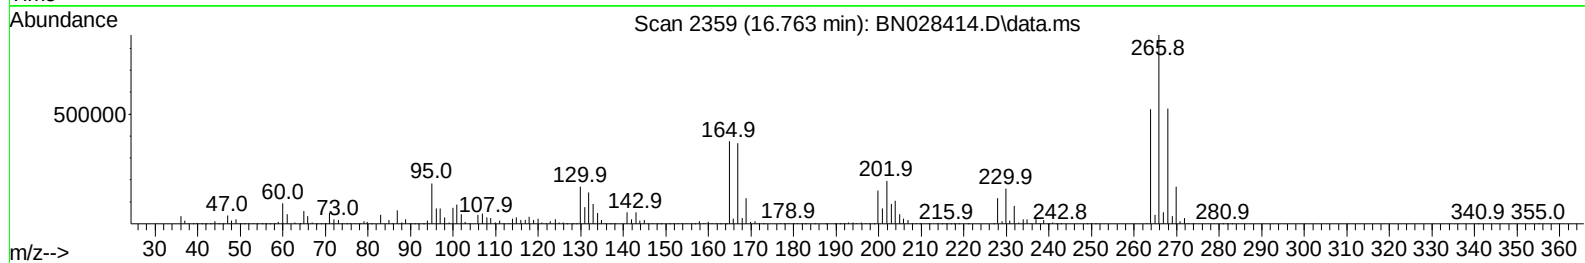


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110223\
Data File : BN028414.D
Acq On : 02 Nov 2023 09:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 06:10:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 06:10:20 2023
Response via : Initial Calibration

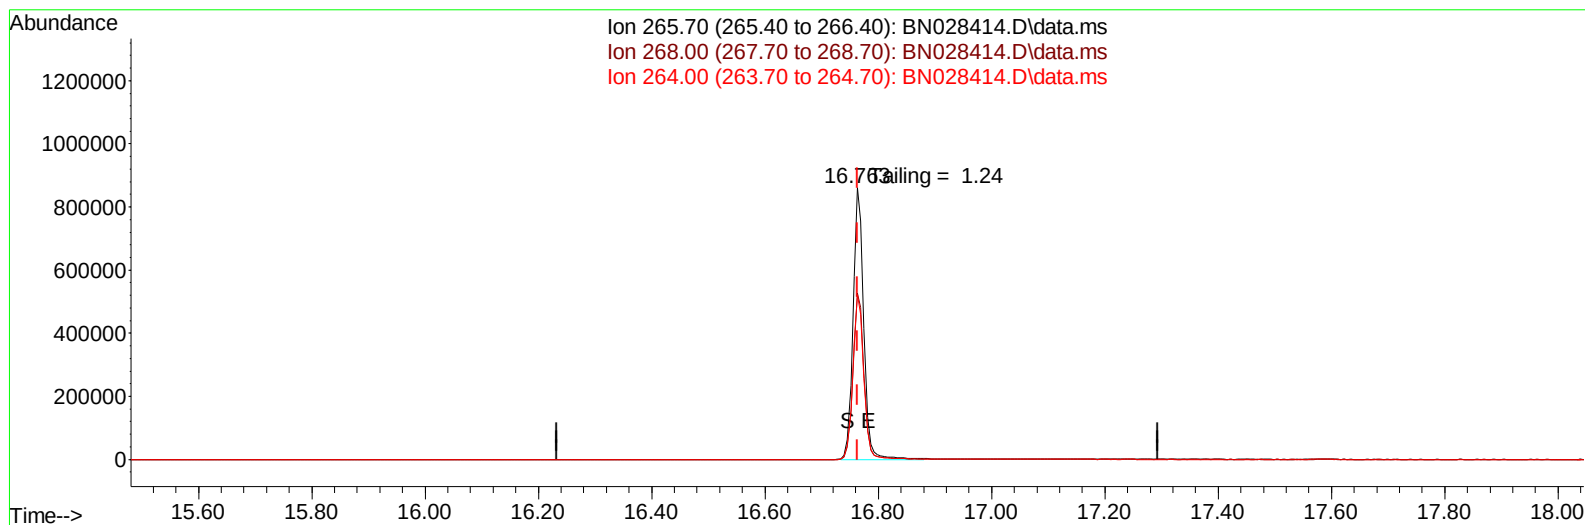

TIC: BN028414.D\data.ms




(70) Pentachlorophenol (C)

16.763min (0.000) 24233.16 ng

response 1142766

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.18
264.00	61.60	60.67
0.00	0.00	0.00

Quant Time: Nov 03 06:10:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 06:10:20 2023
Response via : Initial Calibration

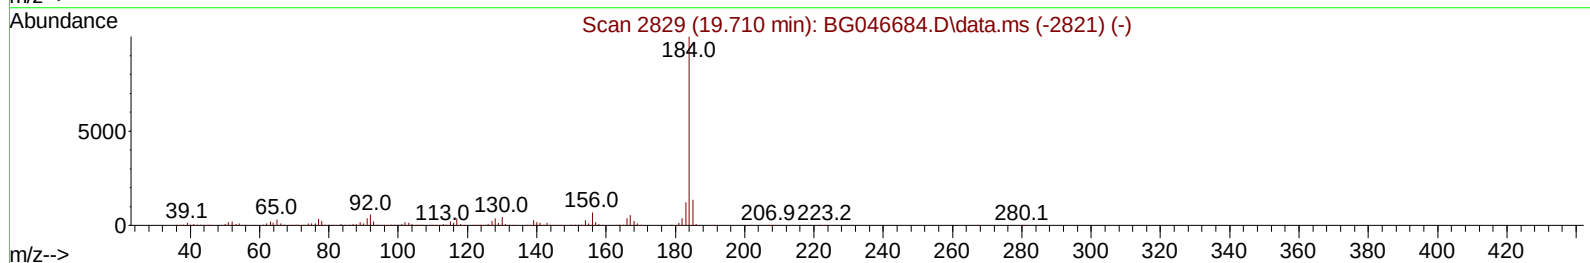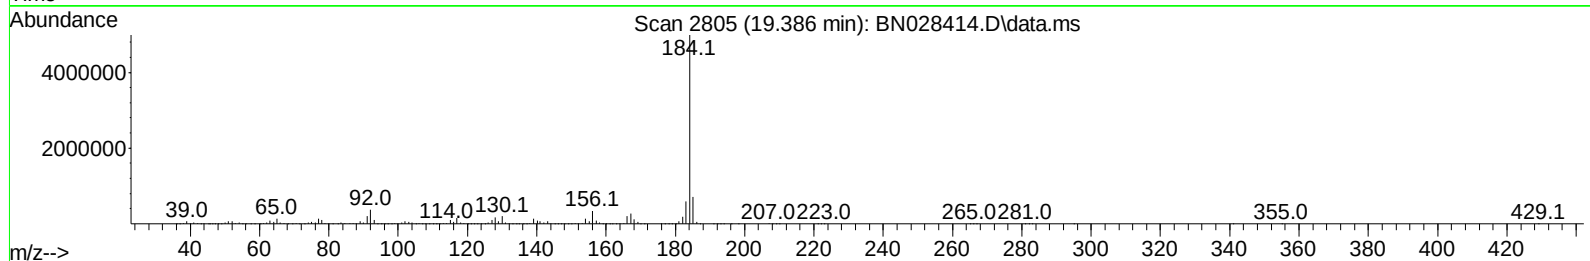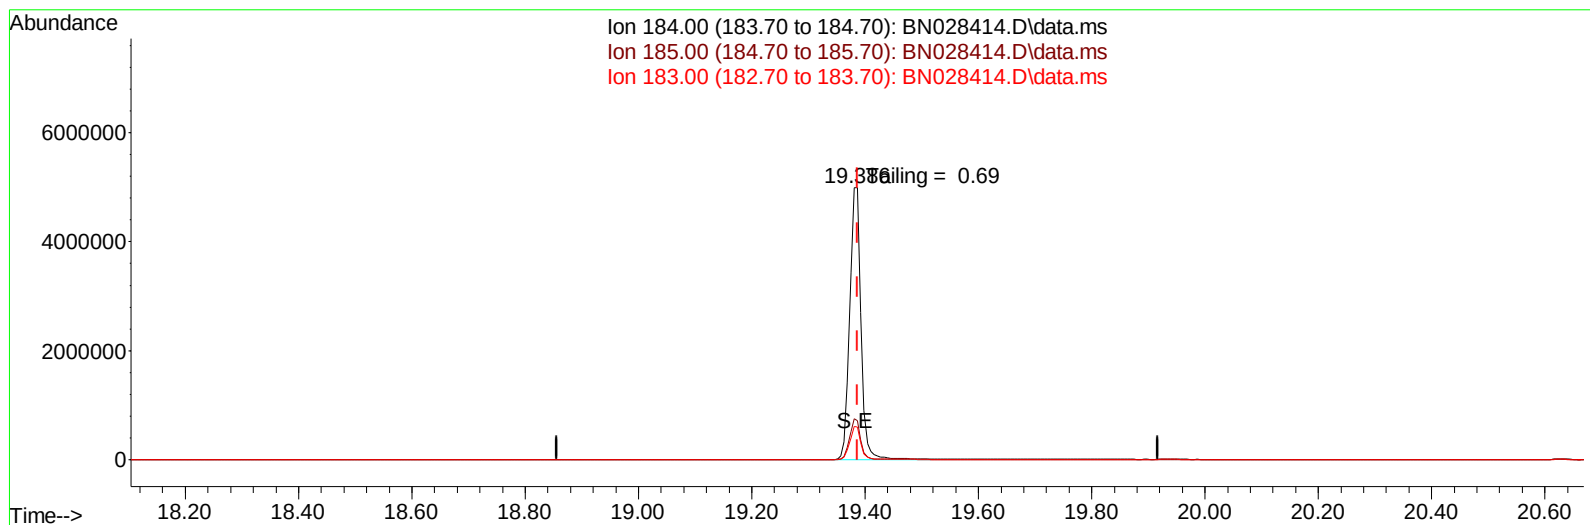

TIC: BN028414.D\data.ms

(77) Benzidine

19.386min (0.000) 0.00 ng

response **6988755**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.20
183.00	13.20	11.91
0.00	0.00	0.00