
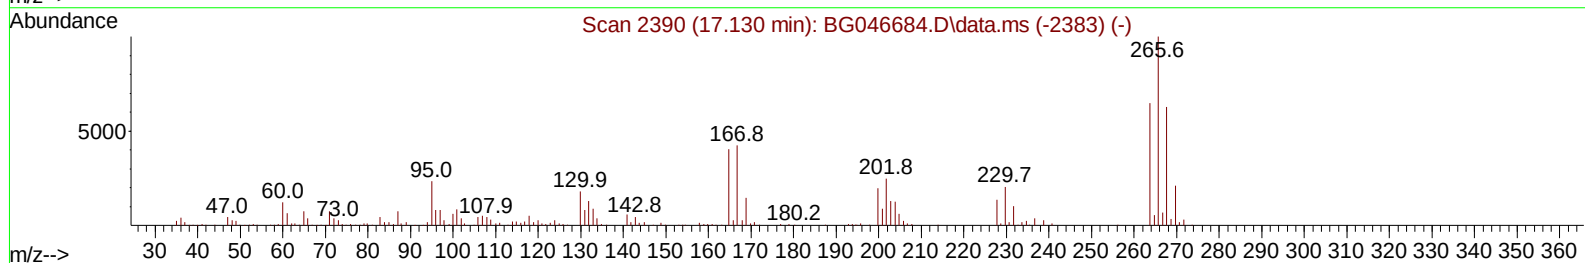
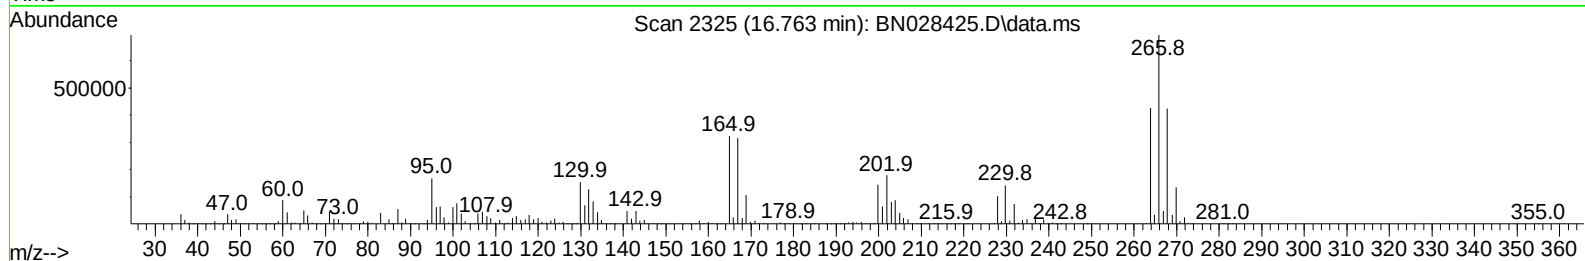


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110223\
Data File : BN028425.D
Acq On : 02 Nov 2023 17:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 06:12:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 06:10:20 2023
Response via : Initial Calibration

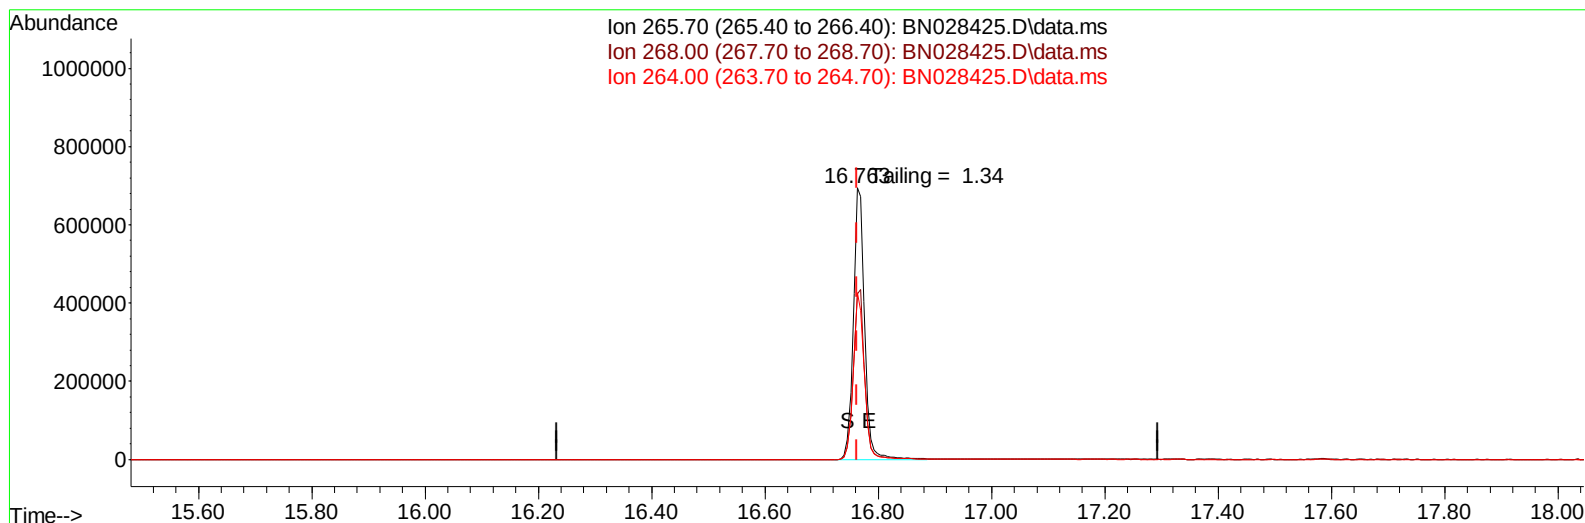

TIC: BN028425.D\data.ms

(70) Pentachlorophenol (C)




16.763min (+ 0.000) 21583.19 ng

response 964108

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.04
264.00	61.60	61.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110223\
Data File : BN028425.D
Acq On : 02 Nov 2023 17:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 06:12:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 06:10:20 2023
Response via : Initial Calibration

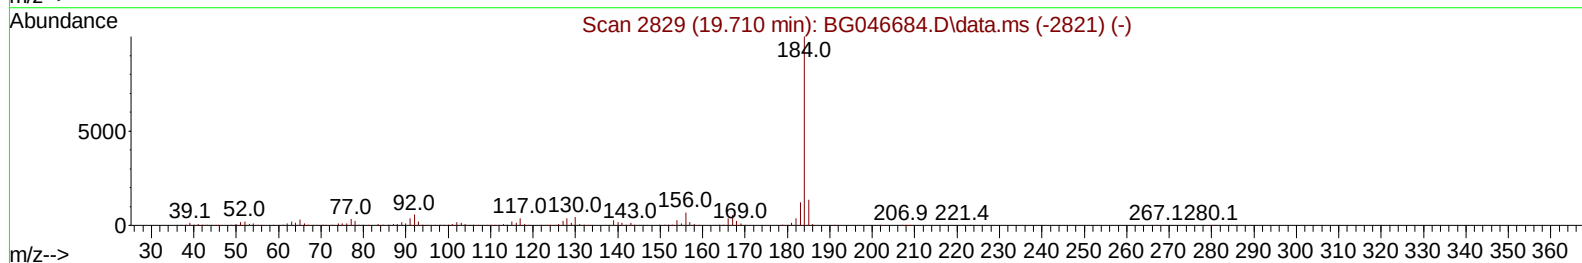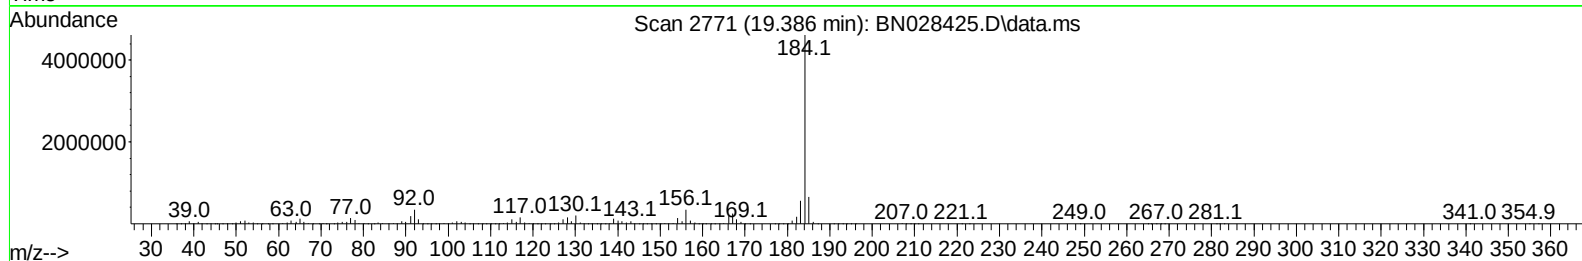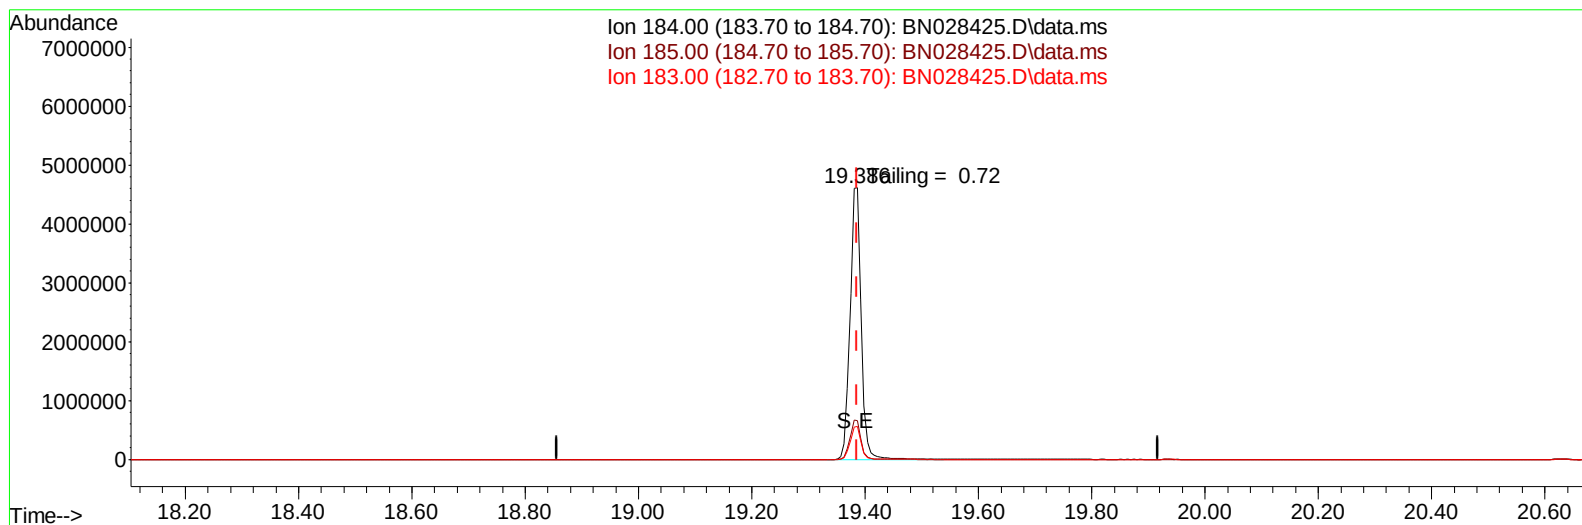

TIC: BN028425.D\data.ms

(77) Benzidine**19.386min (+ 0.000) 0.00 ng****response 6375105**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.25
183.00	13.20	12.19
0.00	0.00	0.00