
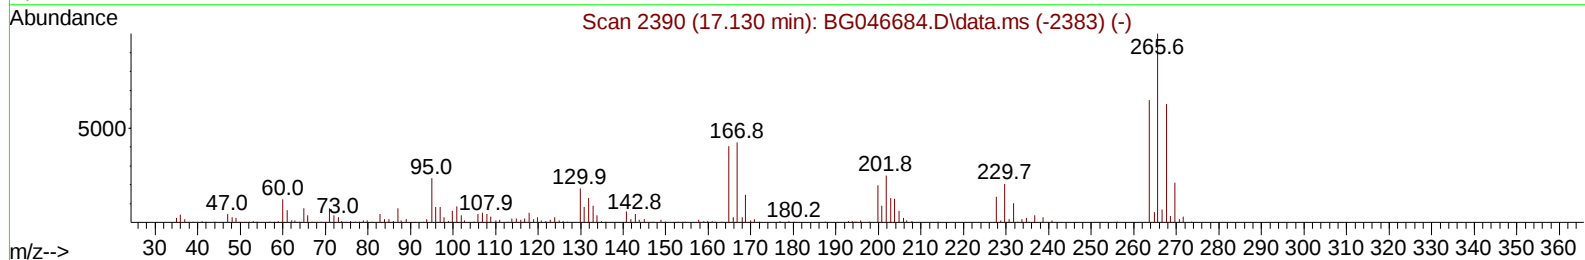
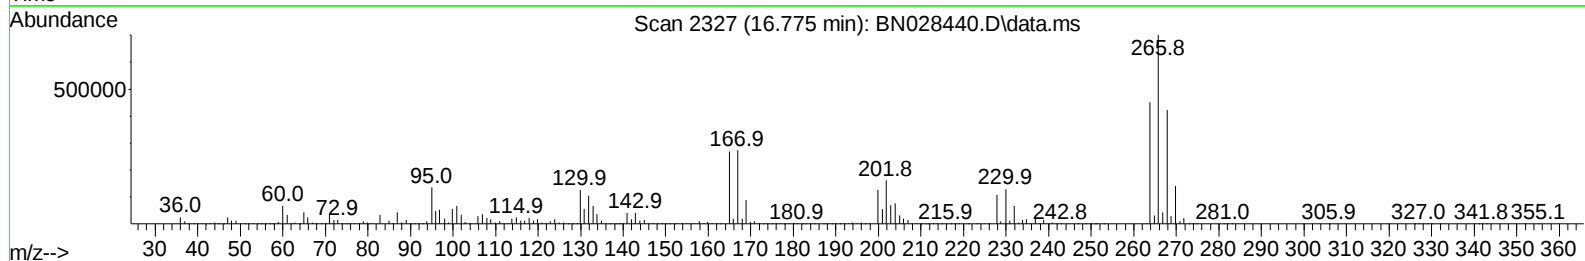


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110223\
Data File : BN028440.D
Acq On : 03 Nov 2023 02:57
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Nov 03 06:13:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 06:10:20 2023
Response via : Initial Calibration

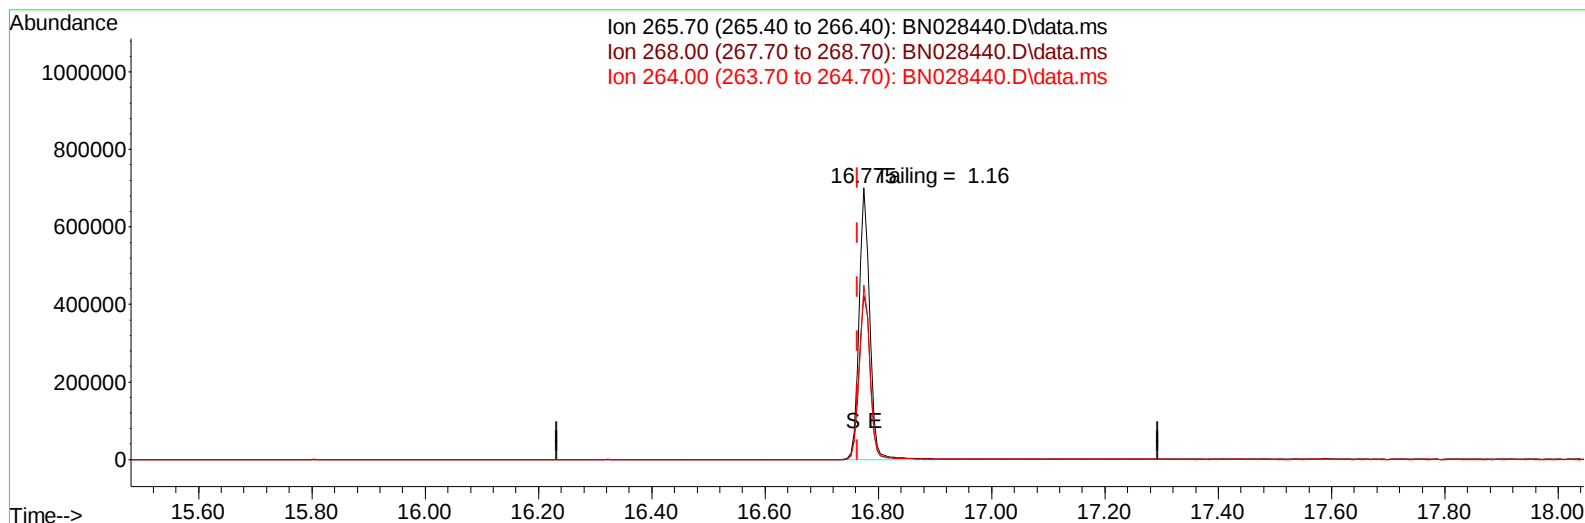

TIC: BN028440.D\data.ms




(70) Pentachlorophenol (C)

16.775min (+ 0.012) 18997.81 ng

response 910642

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.40
264.00	61.60	64.32
0.00	0.00	0.00

Quant Time: Nov 03 06:13:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 06:10:20 2023
Response via : Initial Calibration

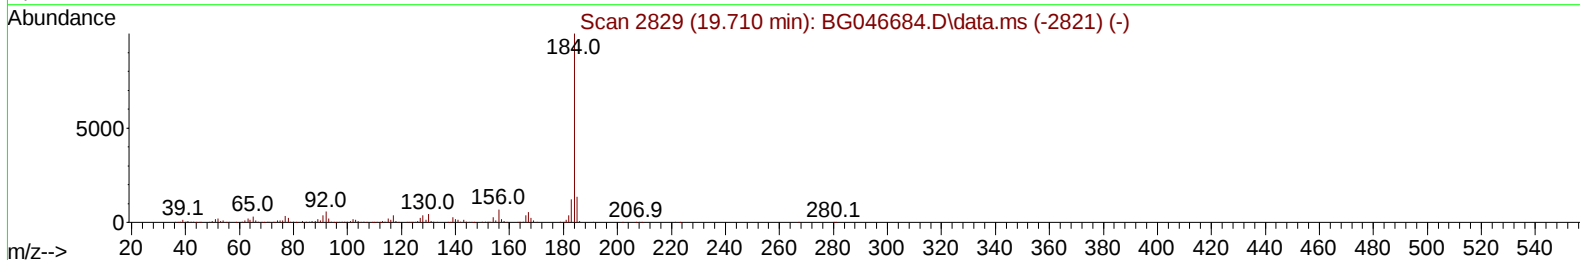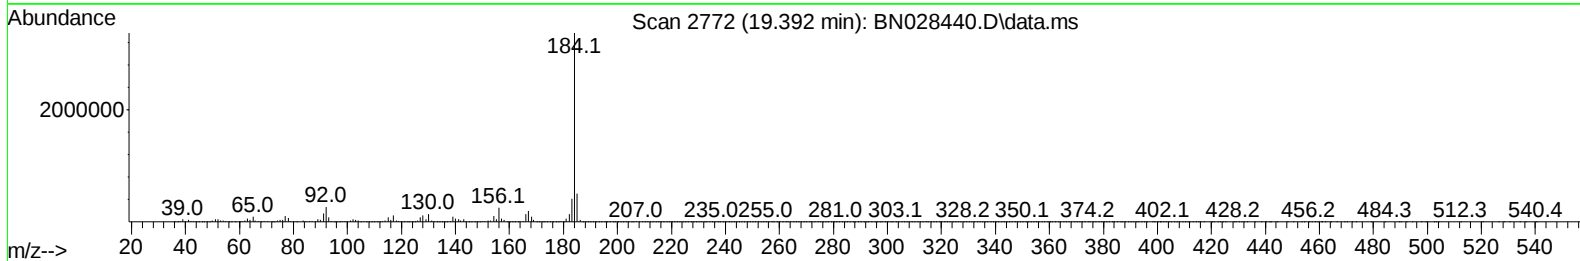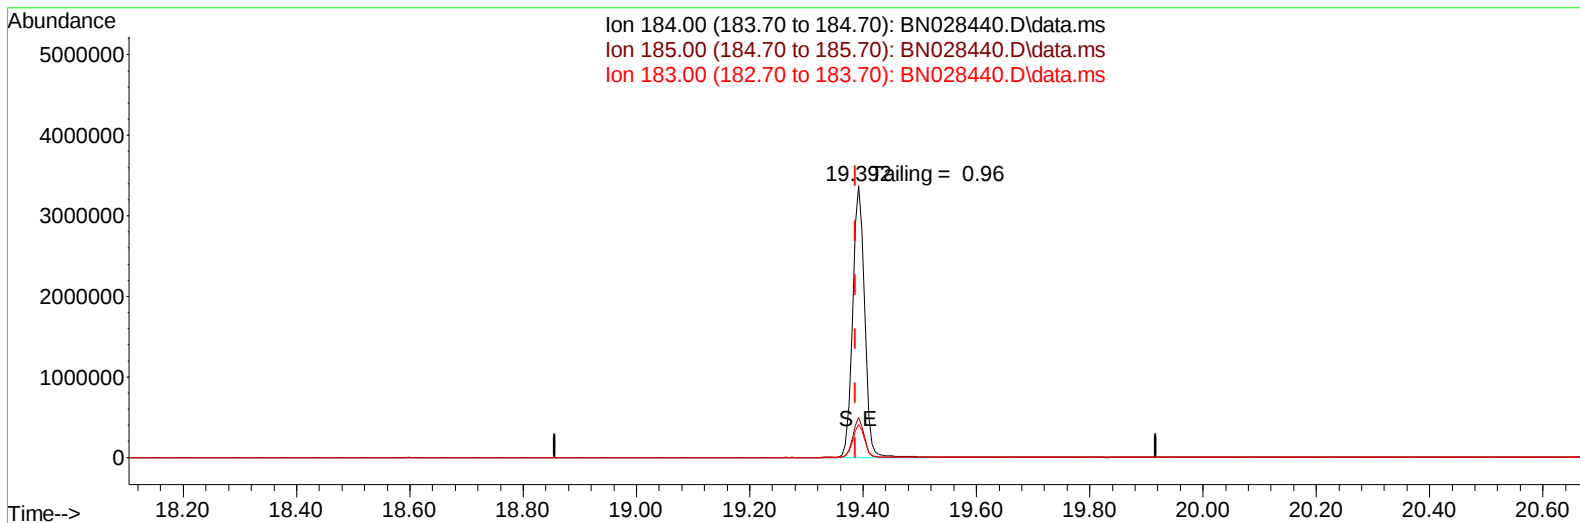

TIC: BN028440.D\data.ms

(77) Benzidine

19.392min (+ 0.006) 138860.11 ng

response **4965281**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.77
183.00	13.20	12.14
0.00	0.00	0.00