


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110223\
Data File : BN028414.D
Acq On : 02 Nov 2023 09:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 02 06:26:50 2023

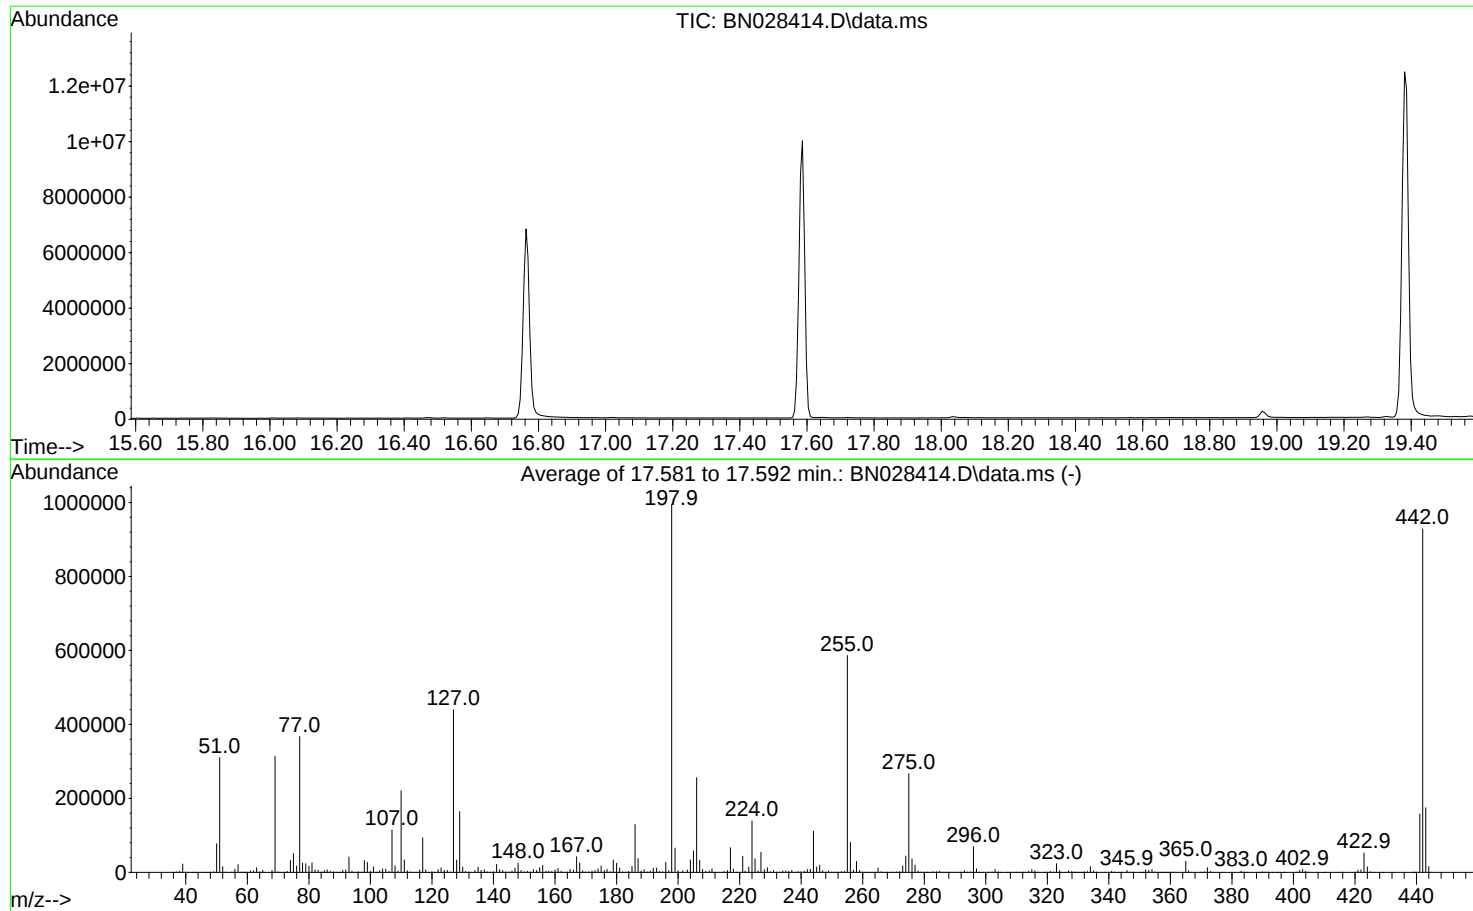




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	310031	PASS
68	69	0.00	2	1.7	5387	PASS
69	198	0.00	100	31.6	314256	PASS
70	69	0.00	2	0.5	1537	PASS
127	198	10	80	44.2	439744	PASS
197	198	0.00	2	0.5	4527	PASS
198	198	100	100	100.0	994709	PASS
199	198	5	9	6.6	65747	PASS
275	198	10	60	26.8	266816	PASS
365	198	1	100	3.0	29925	PASS
441	198	0.01	100	15.9	158099	PASS
442	442	50	100	100.0	928619	PASS
443	442	15	24	18.8	174741	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110223\
Data File : BN028414.D
Acq On : 02 Nov 2023 09:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 03 06:10:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 06:10:20 2023
Response via : Initial Calibration

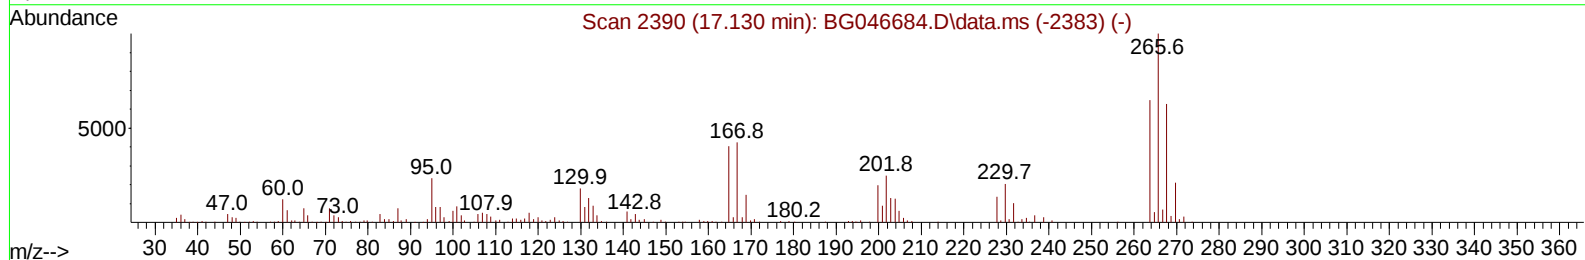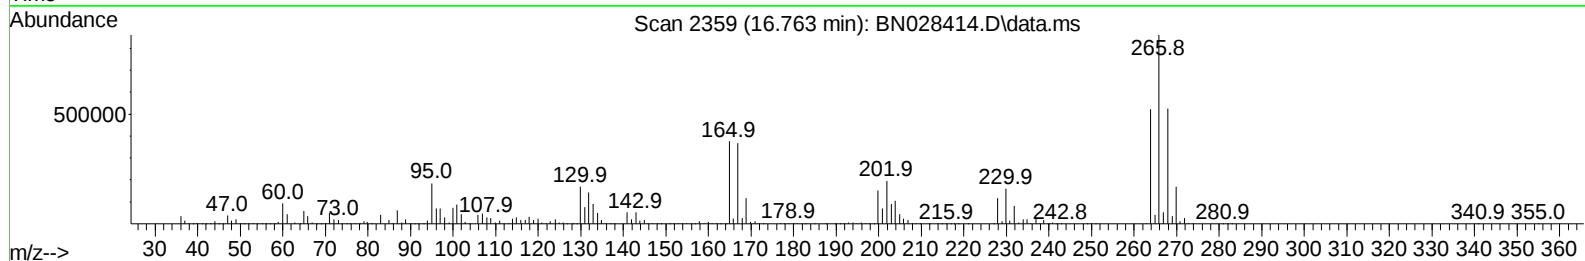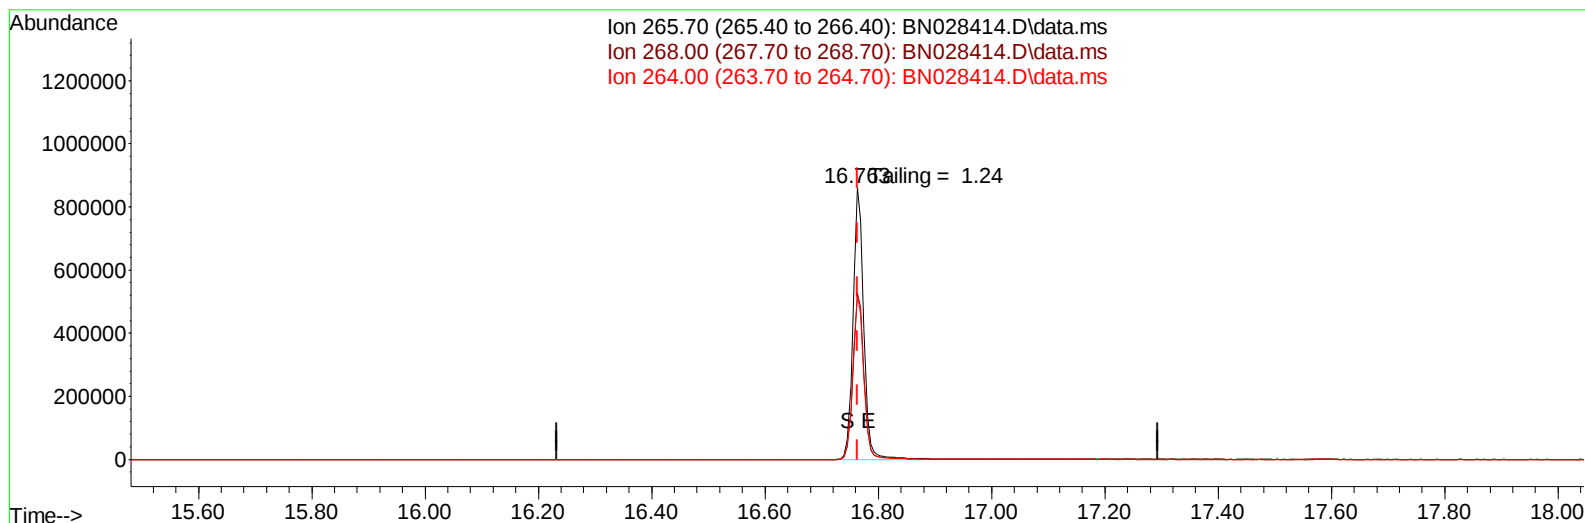

TIC: BN028414.D\data.ms

(70) Pentachlorophenol (C)

16.763min (0.000) 24233.16 ng




response 1142766

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.18
264.00	61.60	60.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110223\
Data File : BN028414.D
Acq On : 02 Nov 2023 09:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 03 06:10:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 06:10:20 2023
Response via : Initial Calibration

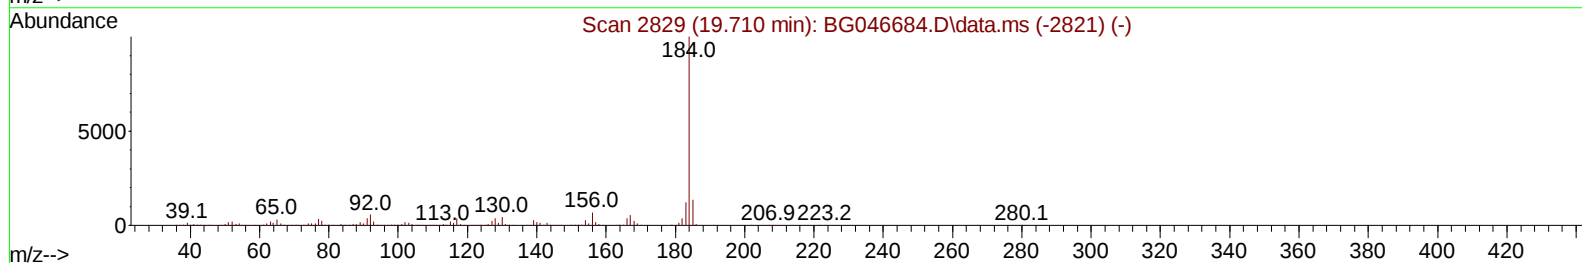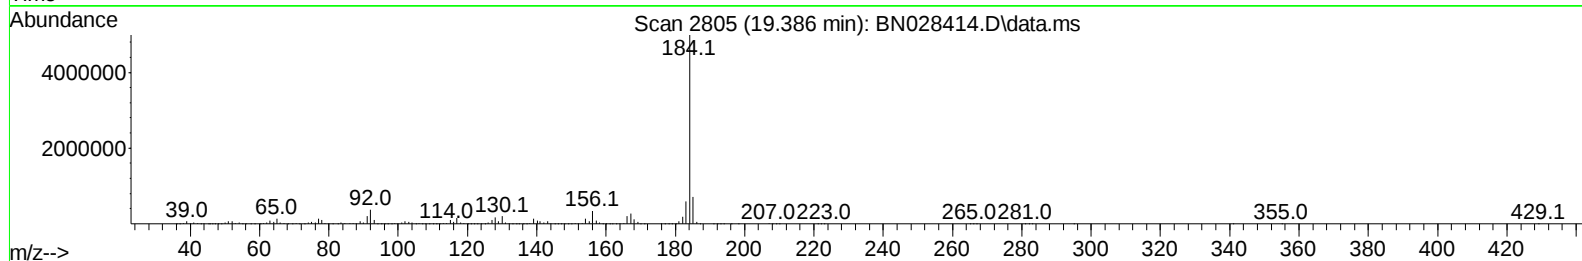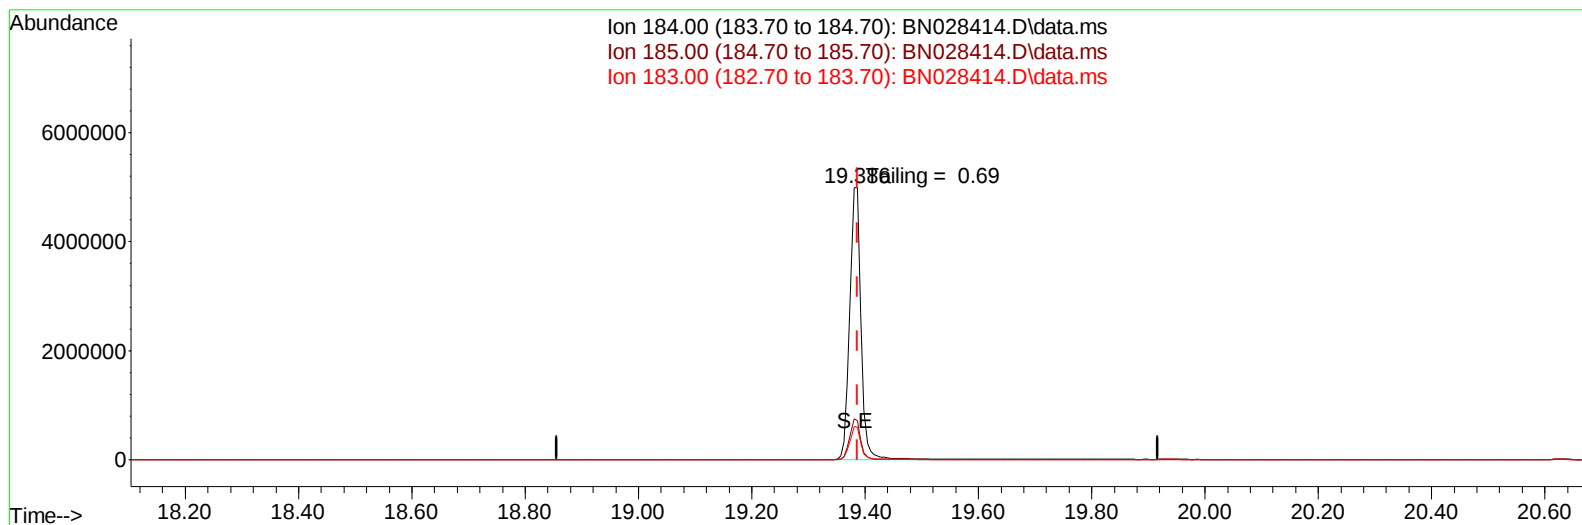

TIC: BN028414.D\data.ms

(77) Benzidine

19.386min (0.000) 0.00 ng

response 6988755

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.20
183.00	13.20	11.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/2/2023	BNA_N	<u>BN028414.D</u>
Compound Name	Response	Retention Time
DDT	3088402	20.627
DDD	244517	20.18
DDE	8847	19.675
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
253364	3341766	7.58

Instrument :
BNA_N
ClientSampleId :
DFTPP