


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110223\
Data File : BN028425.D
Acq On : 02 Nov 2023 17:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 02 06:26:50 2023

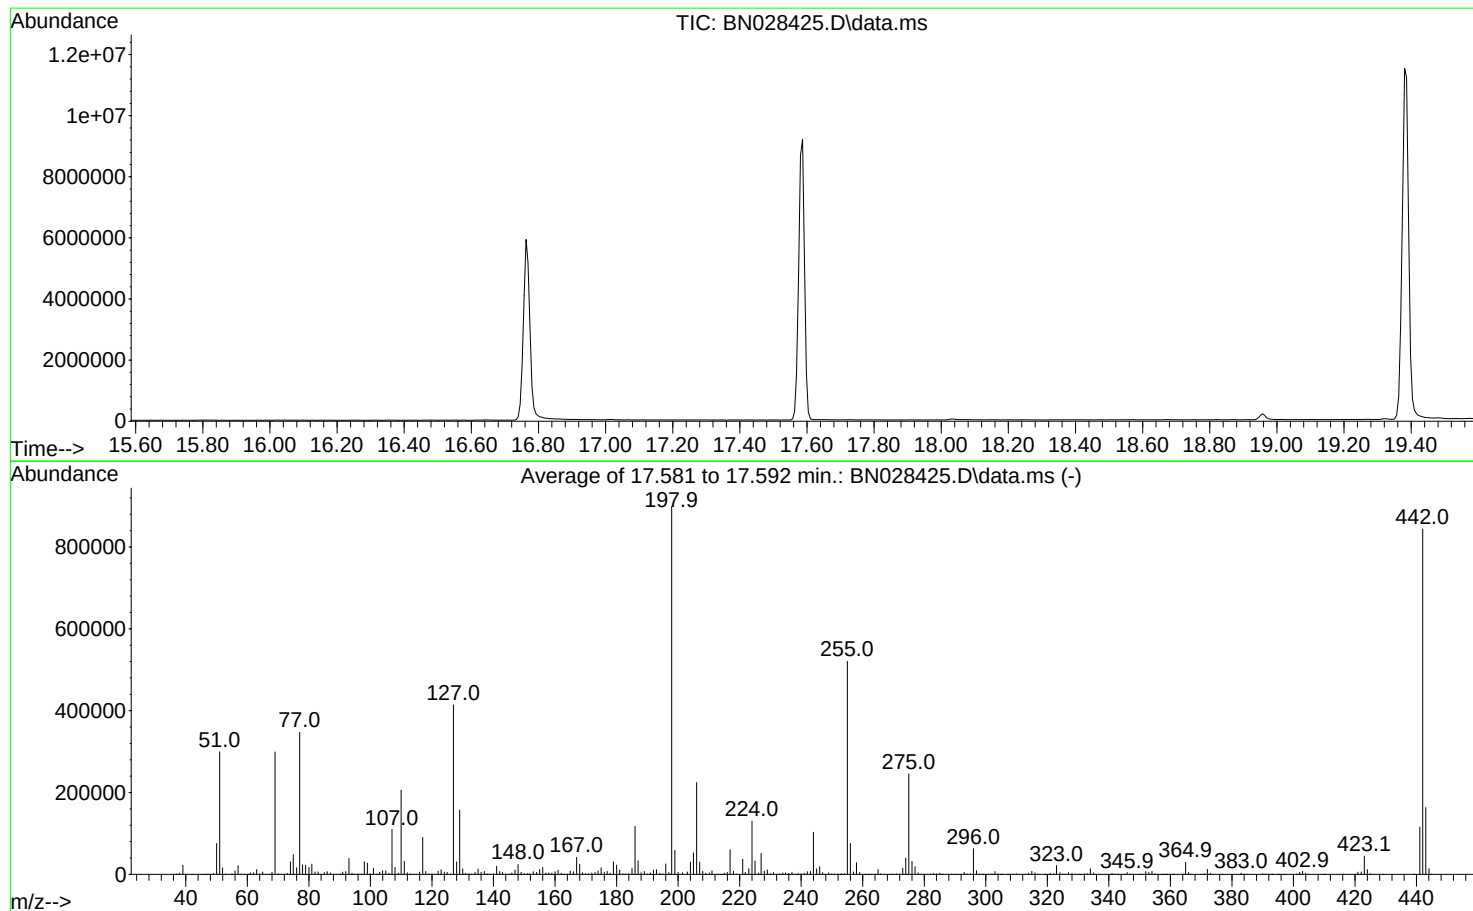




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2456

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	33.3	299706	PASS
68	69	0.00	2	1.7	4950	PASS
69	198	0.00	100	33.3	299051	PASS
70	69	0.00	2	0.5	1592	PASS
127	198	10	80	46.1	414187	PASS
197	198	0.00	2	0.5	4157	PASS
198	198	100	100	100.0	898965	PASS
199	198	5	9	6.5	58760	PASS
275	198	10	60	27.3	245440	PASS
365	198	1	100	3.3	29347	PASS
441	198	0.01	100	12.9	115659	PASS
442	442	50	100	100.0	844011	PASS
443	442	15	24	19.3	163200	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110223\
Data File : BN028425.D
Acq On : 02 Nov 2023 17:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 03 06:12:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 06:10:20 2023
Response via : Initial Calibration

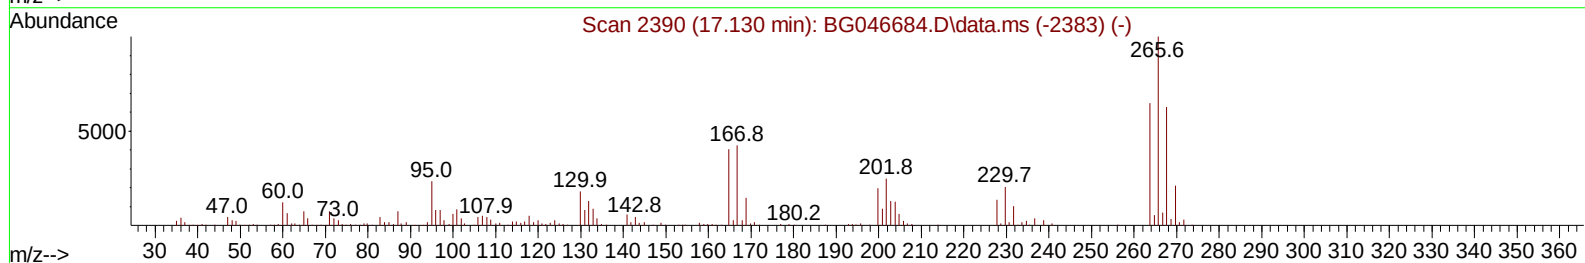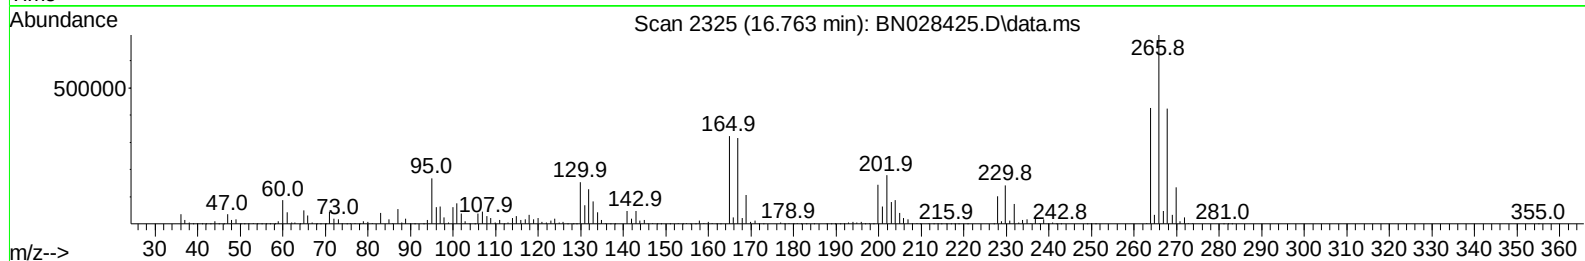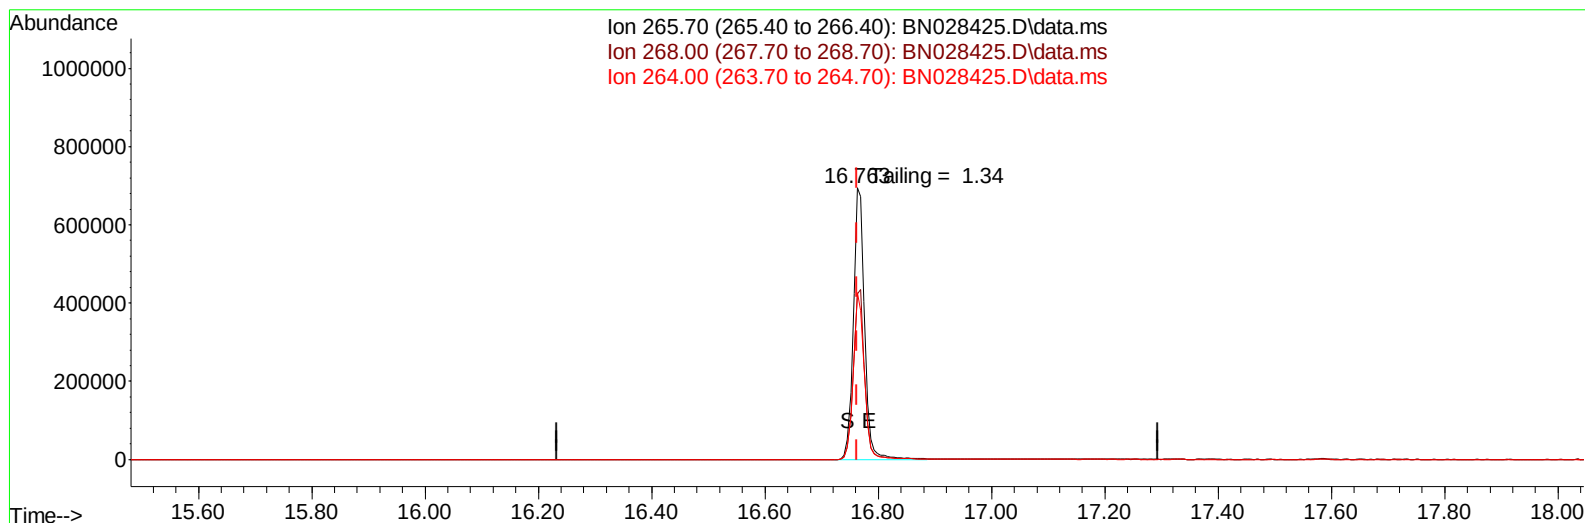

TIC: BN028425.D\data.ms

(70) Pentachlorophenol (C)

16.763min (+ 0.000) 21583.19 ng

response 964108

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.04
264.00	61.60	61.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/2/2023	BNA_N	<u>BN028425.D</u>
Compound Name	Response	Retention Time
DDT	2937614	20.633
DDD	152052	20.186
DDE	5689	19.675
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
157741	3095355	5.10

Instrument :
BNA_N
ClientSampleId :
DFTPP