


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110223\
 Data File : BN028440.D
 Acq On : 03 Nov 2023 02:57
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 02 06:26:50 2023

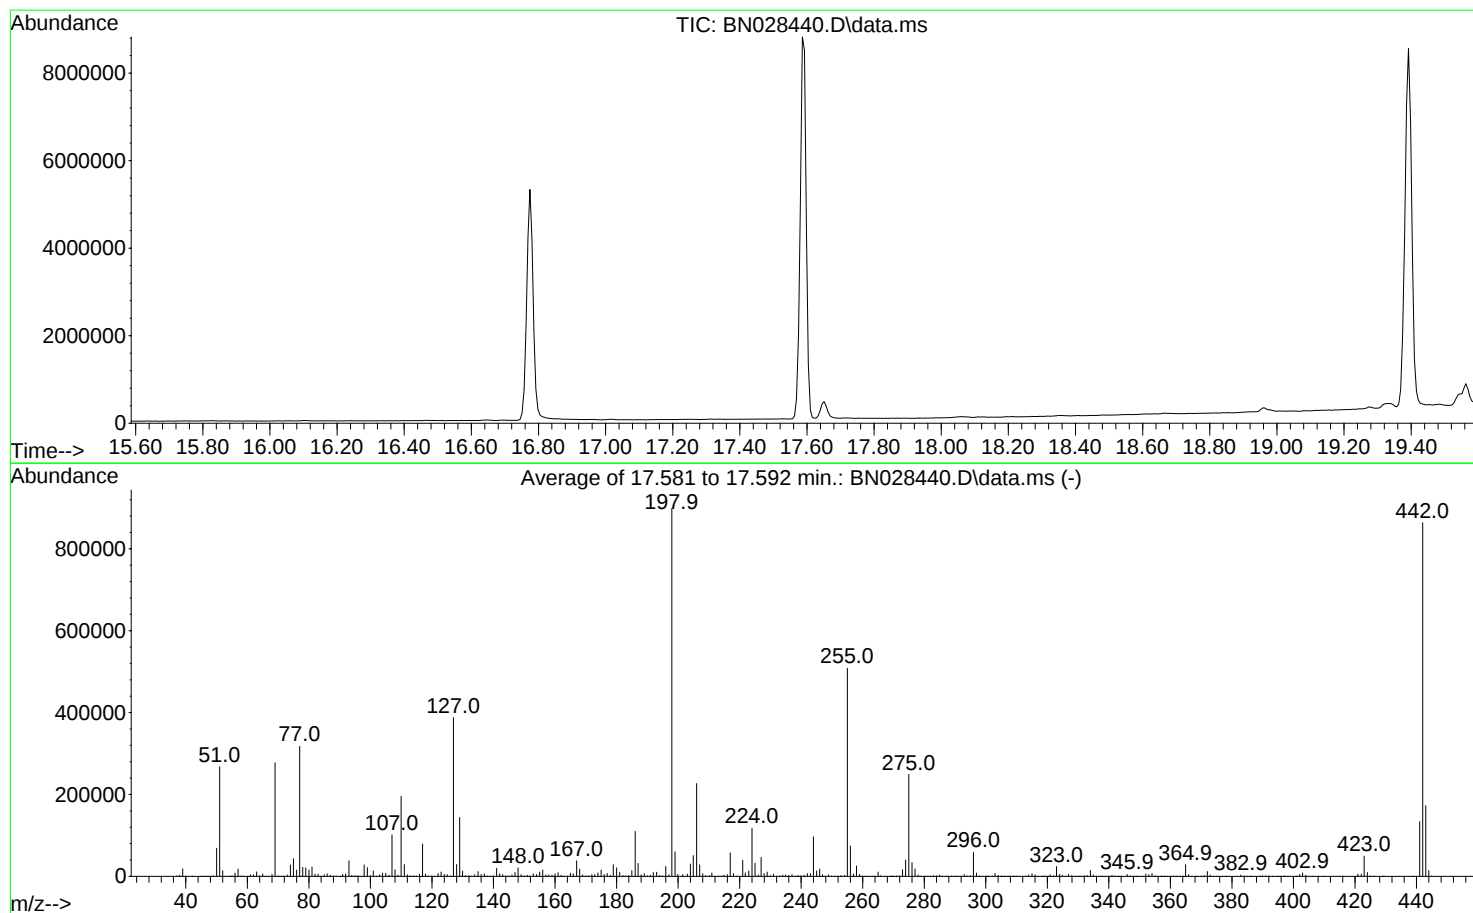




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	267839	PASS
68	69	0.00	2	1.7	4635	PASS
69	198	0.00	100	30.9	277389	PASS
70	69	0.00	2	0.4	1175	PASS
127	198	10	80	43.1	387574	PASS
197	198	0.00	2	0.4	3966	PASS
198	198	100	100	100.0	898453	PASS
199	198	5	9	6.6	59693	PASS
275	198	10	60	27.7	248811	PASS
365	198	1	100	3.2	28549	PASS
441	198	0.01	100	14.9	133483	PASS
442	442	50	100	100.0	863765	PASS
443	442	15	24	20.0	172917	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110223\
Data File : BN028440.D
Acq On : 03 Nov 2023 02:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 03 06:13:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 06:10:20 2023
Response via : Initial Calibration

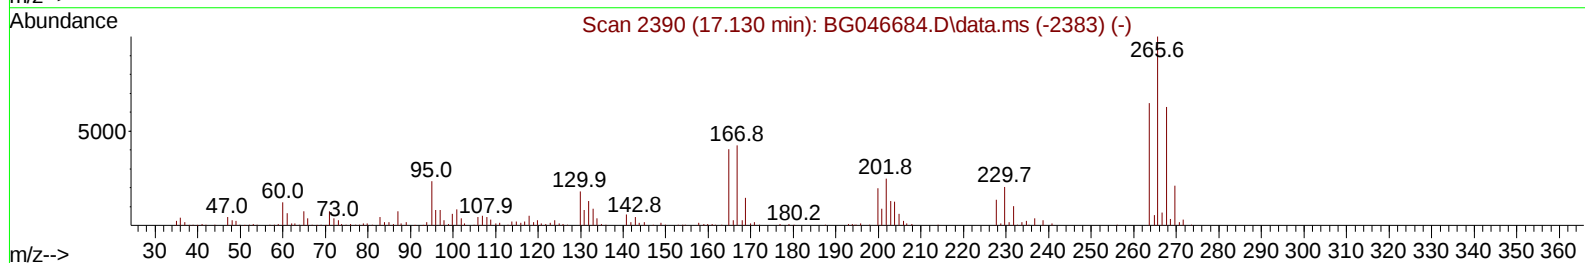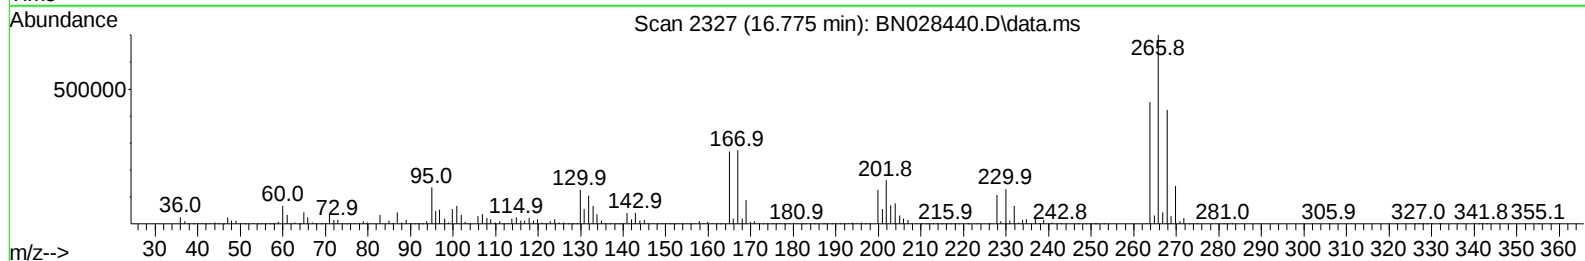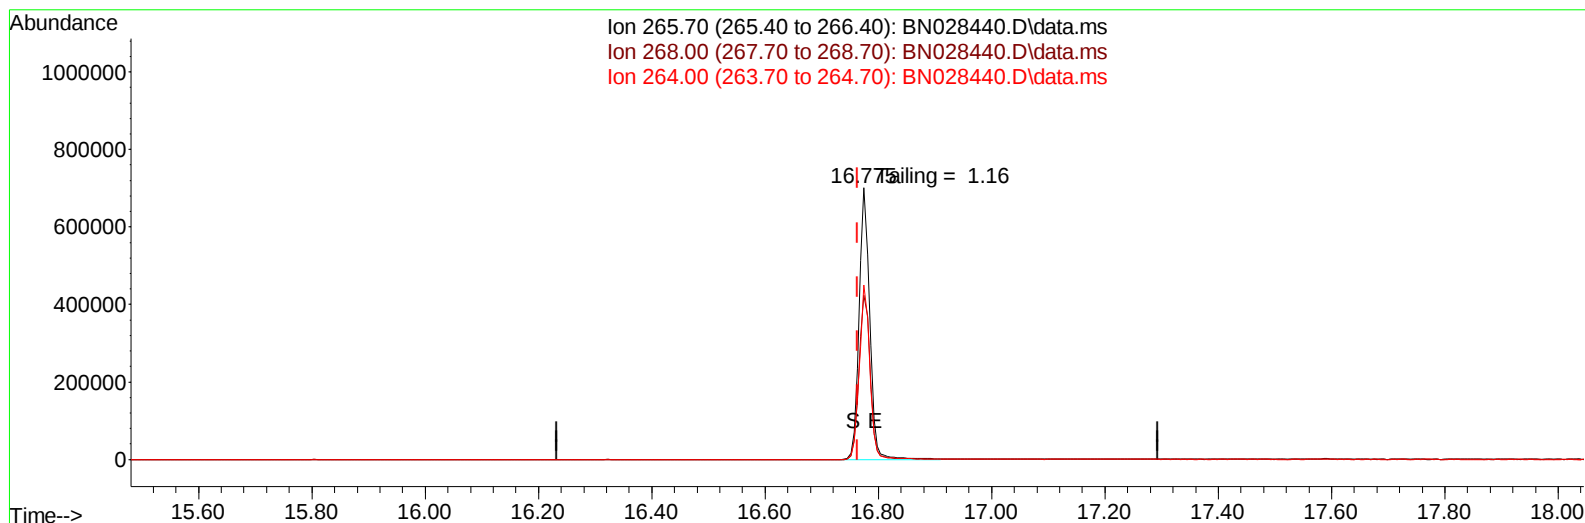

TIC: BN028440.D\data.ms

(70) Pentachlorophenol (C)

16.775min (+ 0.012) 18997.81 ng

response 910642

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.40
264.00	61.60	64.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/2/2023	BNA_N	<u>BN028440.D</u>
Compound Name	Response	Retention Time
DDT	74316	20.633
DDD	1105463	20.192
DDE	2243	19.675
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1107706	1182022	93.71

Instrument :
BNA_N
ClientSampleId :
DFTPP