
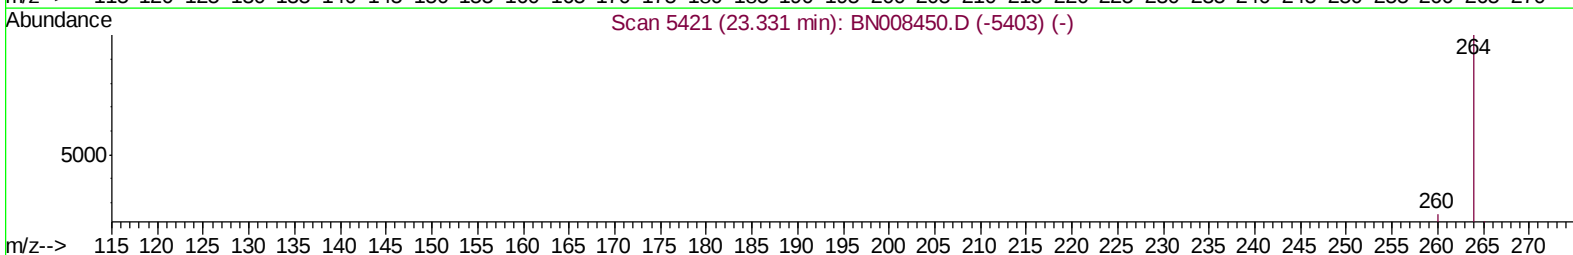
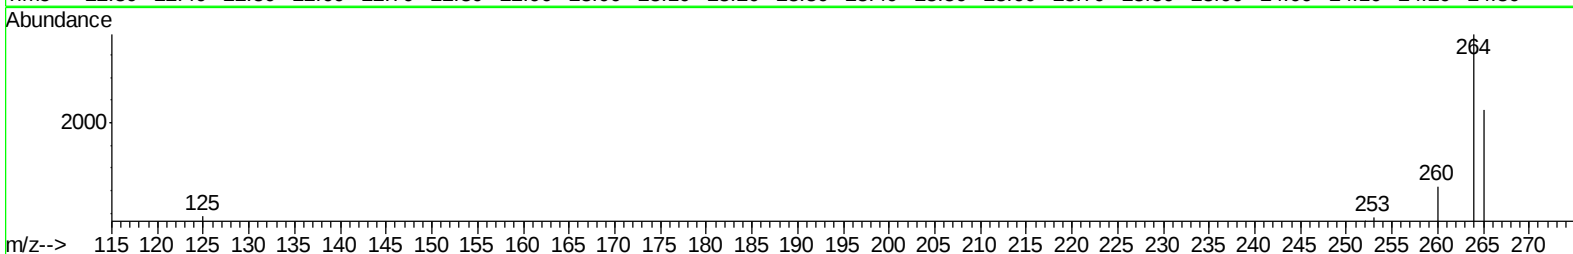


Data File : BN008451.D
Acq On : 05 Nov 2019 17:37
Operator : JU
Sample : K5567-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Nov 06 01:15:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 00:56:29 2019
Response via : Initial Calibration

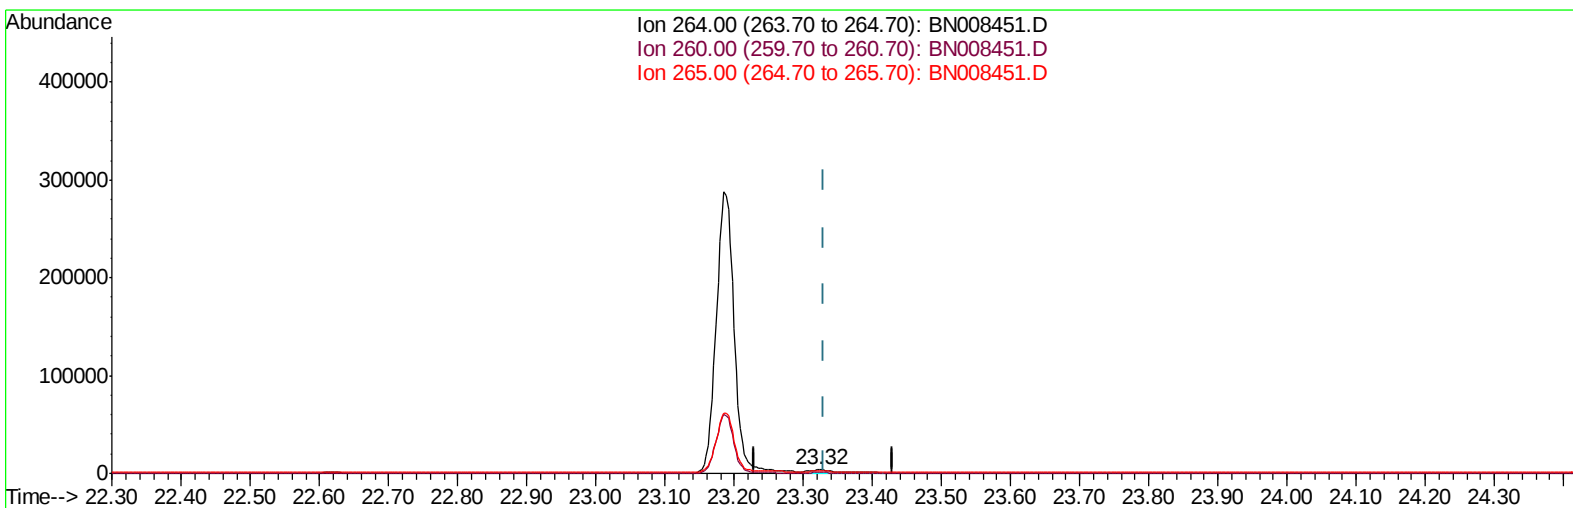

TIC: BN008451.D

(20) Perylene-d12 (I)

23.323min (-0.008) 0.40ng/ul

response 7053

Ion	Exp%	Act%
264.00	100	100
260.00	41.20	24.77#
265.00	712.80	62.58#
0.00	0.00	0.00