
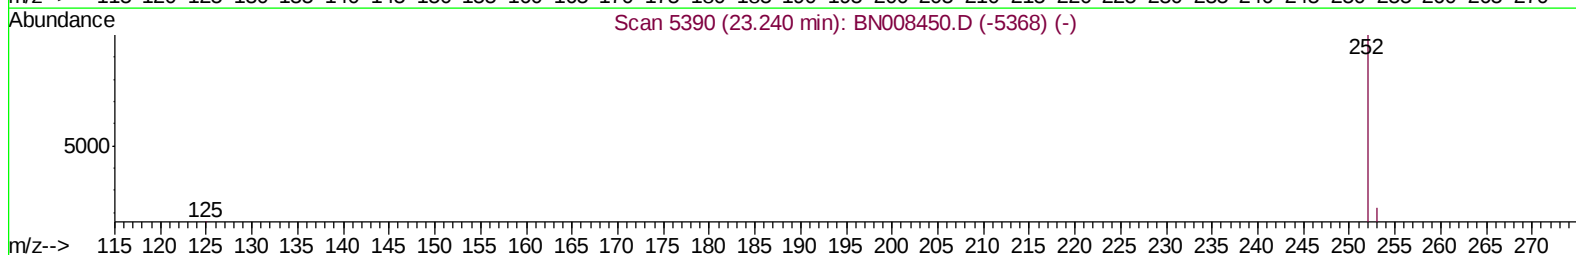
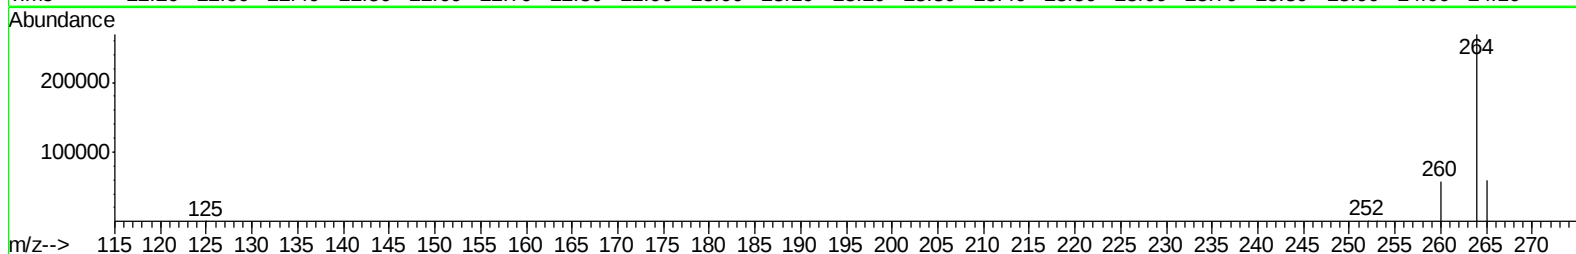


Data File : BN008451.D
Acq On : 05 Nov 2019 17:37
Operator : JU
Sample : K5567-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Nov 06 01:16:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 00:56:29 2019
Response via : Initial Calibration

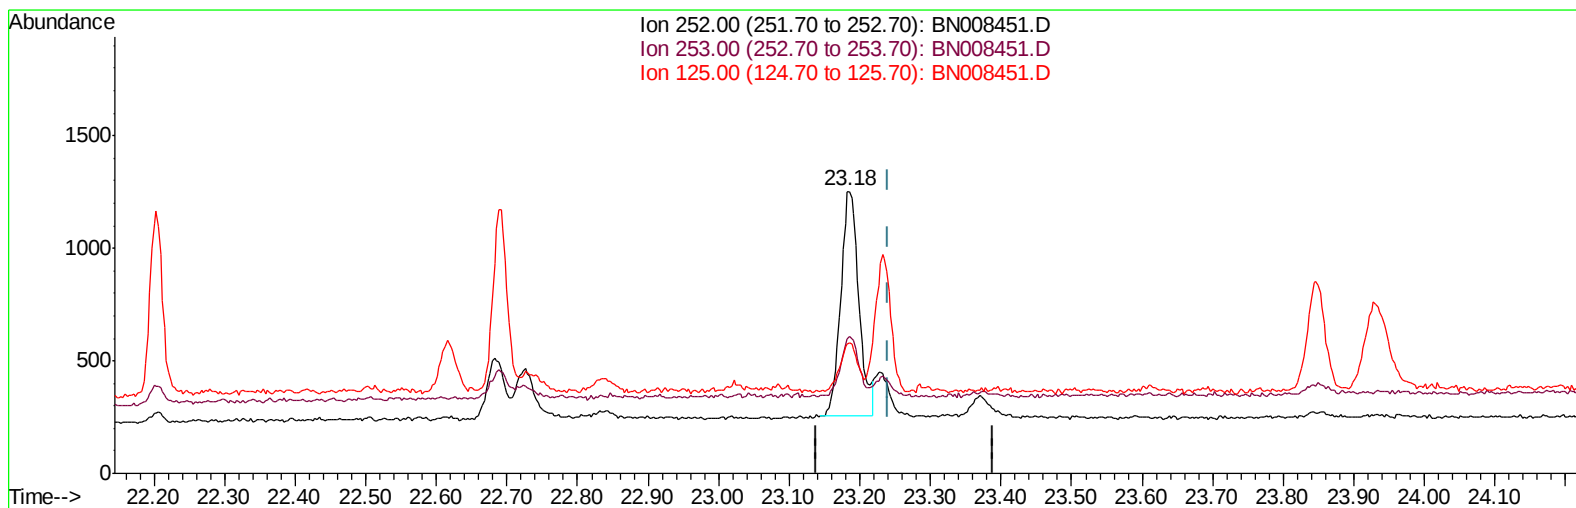

TIC: BN008451.D

(23) Benzo(a)pyrene (C)
23.182min (-0.058) 0.13ng/ul
response 1788

Ion	Exp%	Act%
252.00	100	100
253.00	33.40	47.72#
125.00	25.70	45.72#
0.00	0.00	0.00