
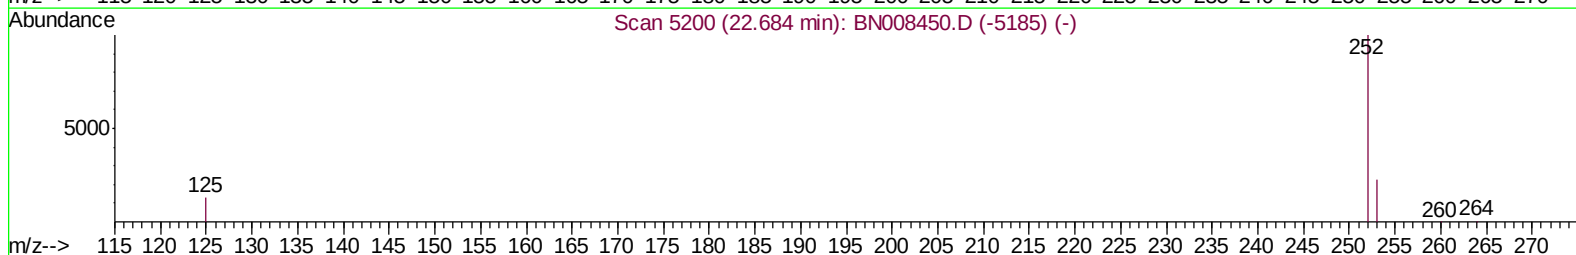
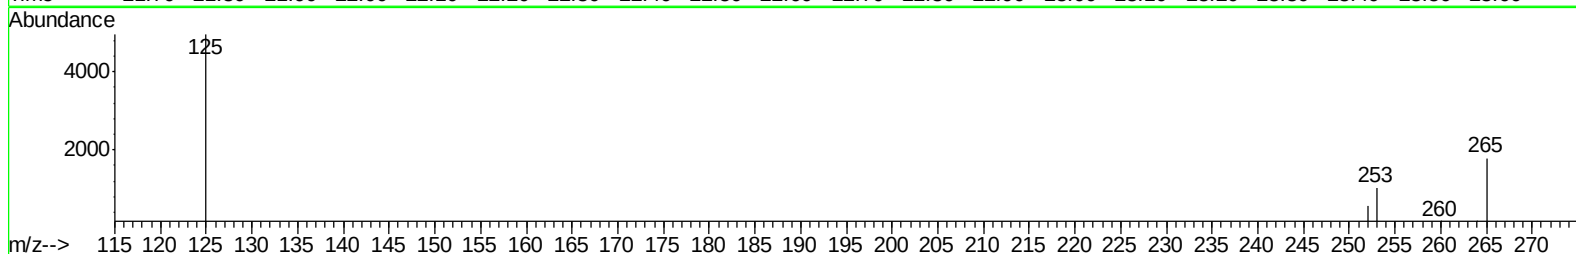


Data File : BN008458.D
Acq On : 05 Nov 2019 21:48
Operator : JU
Sample : K5567-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Nov 06 02:55:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 00:56:29 2019
Response via : Initial Calibration

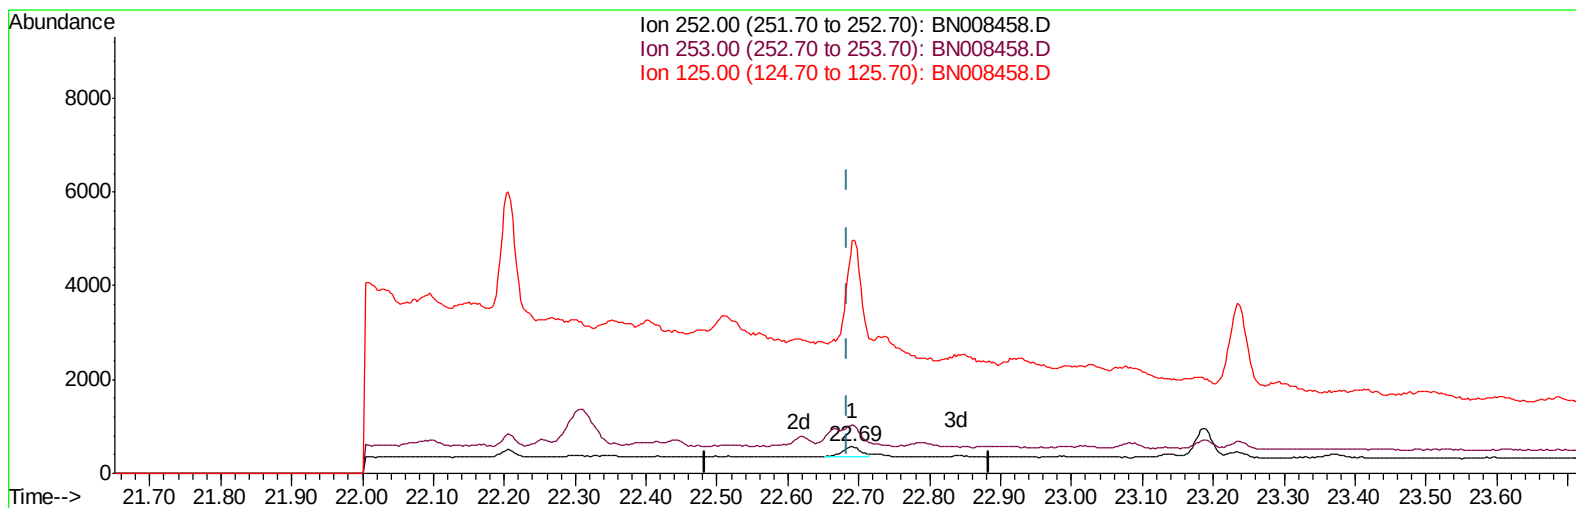

TIC: BN008458.D

(21) Benzo(b)fluoranthene

22.691min (+0.007) 0.04ng/ul m

response 410

Ion	Exp%	Act%
252.00	100	100
253.00	29.80	182.01#
125.00	20.00	873.90#
0.00	0.00	0.00