
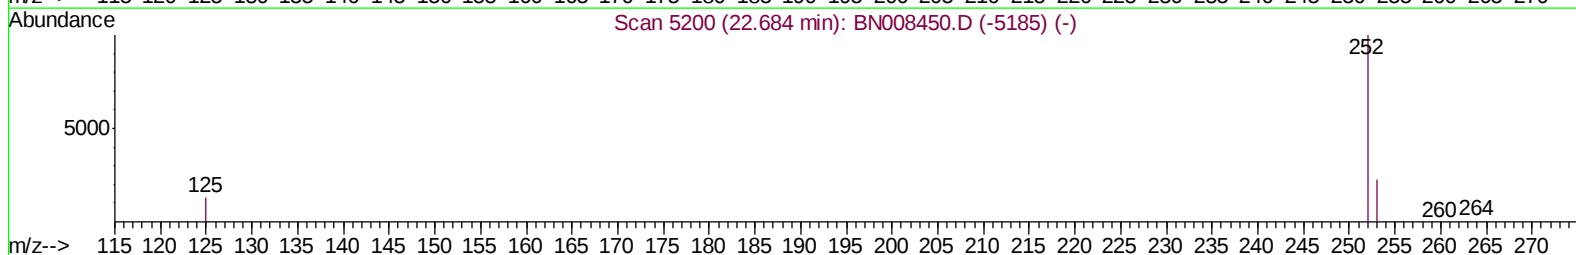
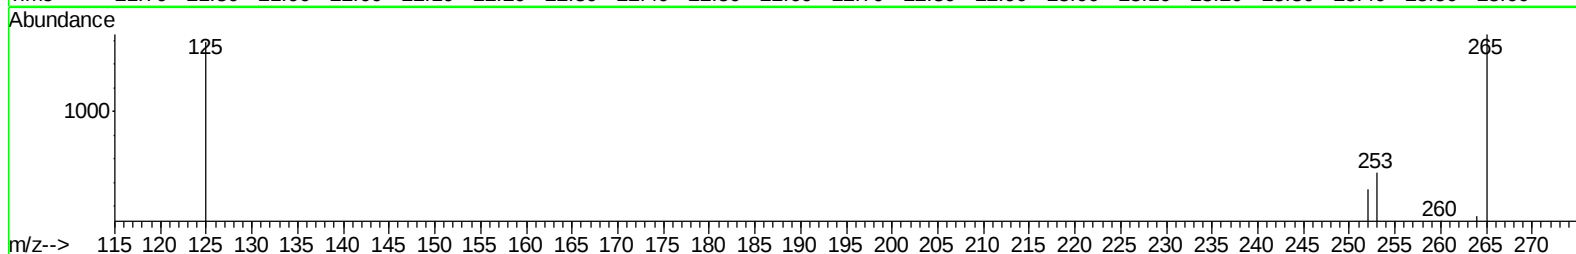


Data File : BN008459.D
Acq On : 05 Nov 2019 22:24
Operator : JU
Sample : K5567-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Nov 06 03:00:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 00:56:29 2019
Response via : Initial Calibration

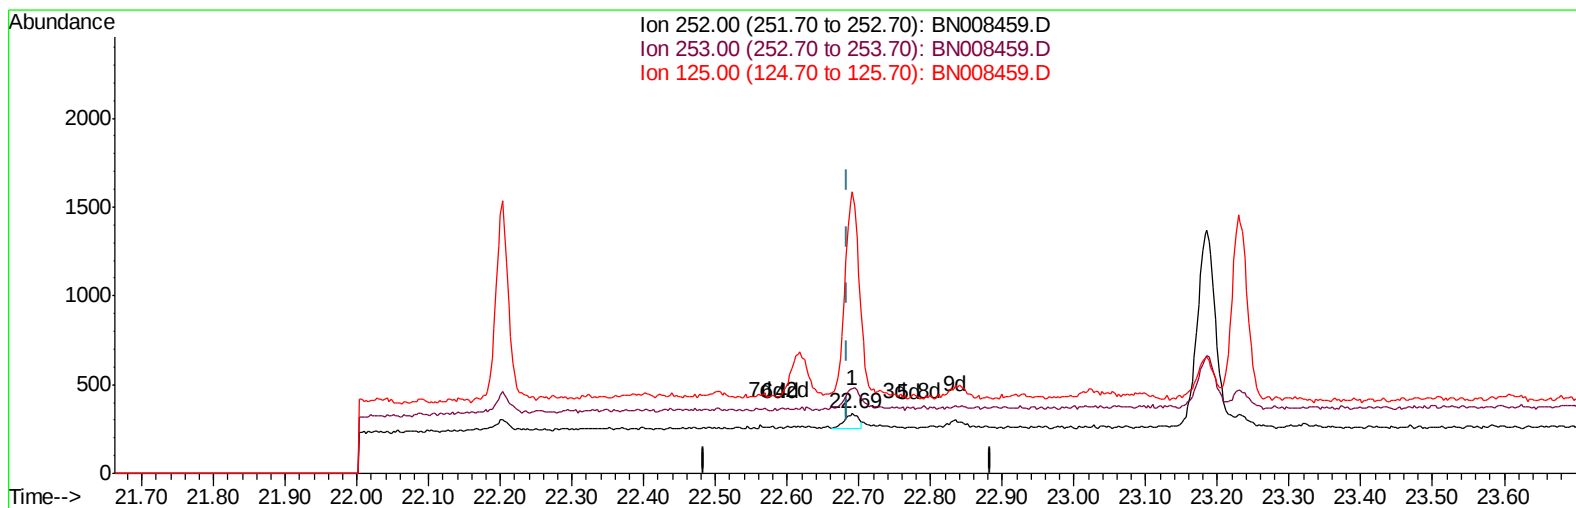

TIC: BN008459.D

(21) Benzo(b)fluoranthene

22.691min (+0.007) 0.03ng/ul m

response 122

Ion	Exp%	Act%
252.00	100	100
253.00	29.80	141.72#
125.00	20.00	469.23#
0.00	0.00	0.00