
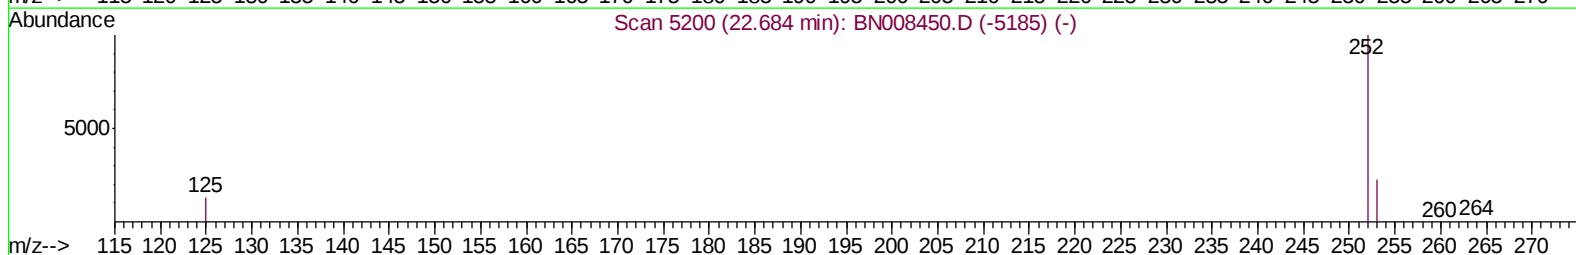
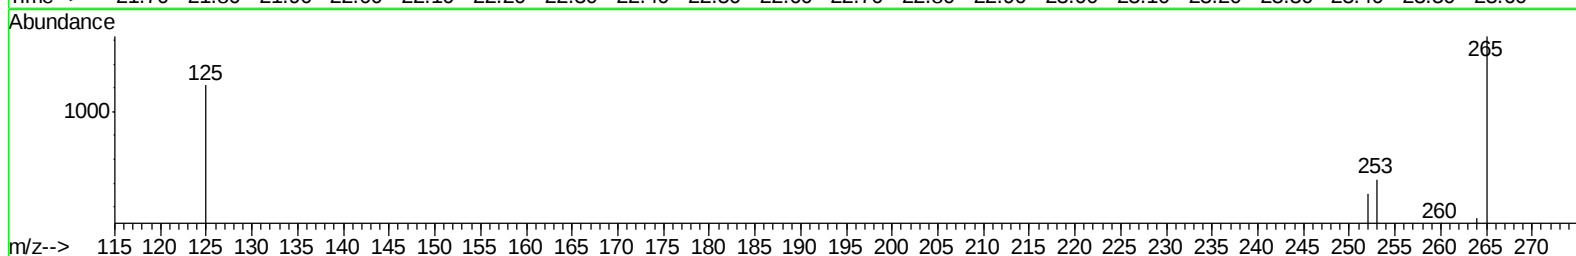


Data File : BN008460.D
Acq On : 05 Nov 2019 23:00
Operator : JU
Sample : K5567-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Nov 06 03:03:25 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 00:56:29 2019
Response via : Initial Calibration

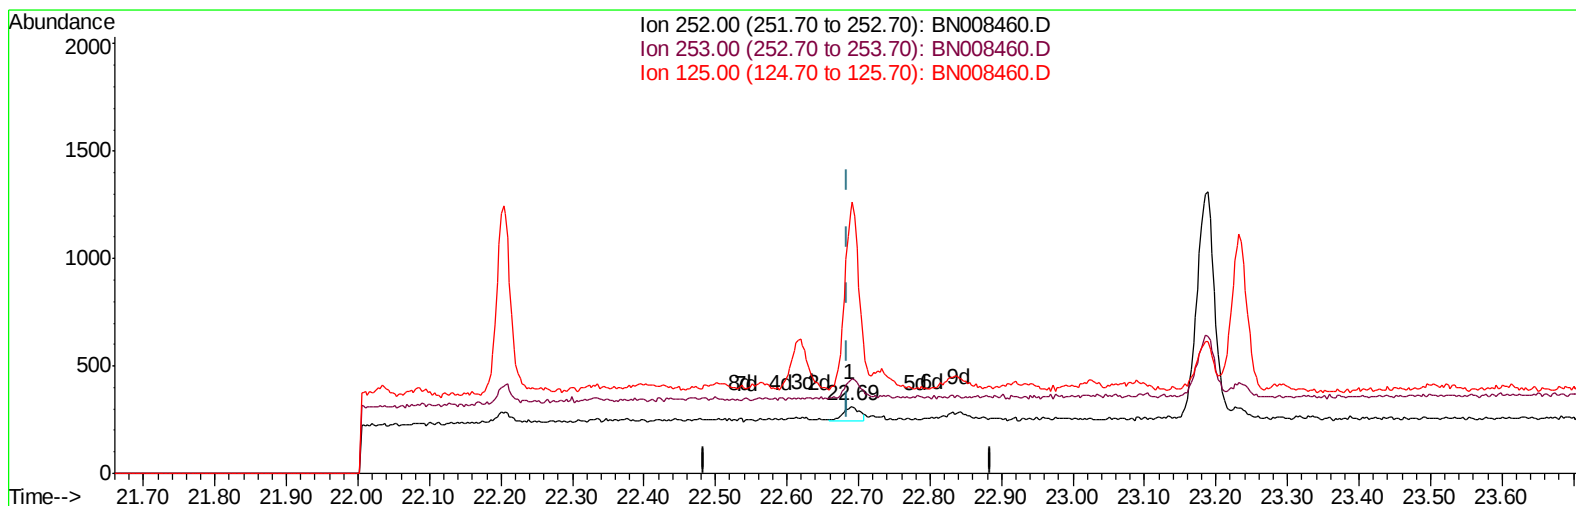

TIC: BN008460.D

(21) Benzo(b)fluoranthene

22.689min (+0.004) 0.03ng/ul m

response 107

Ion	Exp%	Act%
252.00	100	100
253.00	29.80	139.68#
125.00	20.00	393.87#
0.00	0.00	0.00