

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110519\
 Data File : BN008452.D
 Acq On : 05 Nov 2019 18:13
 Operator : JU
 Sample : K5567-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Nov 07 11:15:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 10:57:49 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	1363	0.40	ng/ul	0.00
2) Naphthalene-d8	10.32	136	5969	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.20	164	3543	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.95
16) Chrysene-d12	21.16	240	5513	0.40	ng/ul	0.00
20) Perylene-d12	23.32	264	6839	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.92	152	2659	0.28	ng/ul	0.00
14) Fluoranthene-d10	18.99	212	8499	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.35	202	1186	0.044	ng/ul#	1
23) Benzo(a)pyrene	23.19	252	1794	0.070	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110519\
Data File : BN008452.D
Acq On : 05 Nov 2019 18:13
Operator : JU
Sample : K5567-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Nov 07 11:15:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 10:57:49 2019
Response via : Initial Calibration

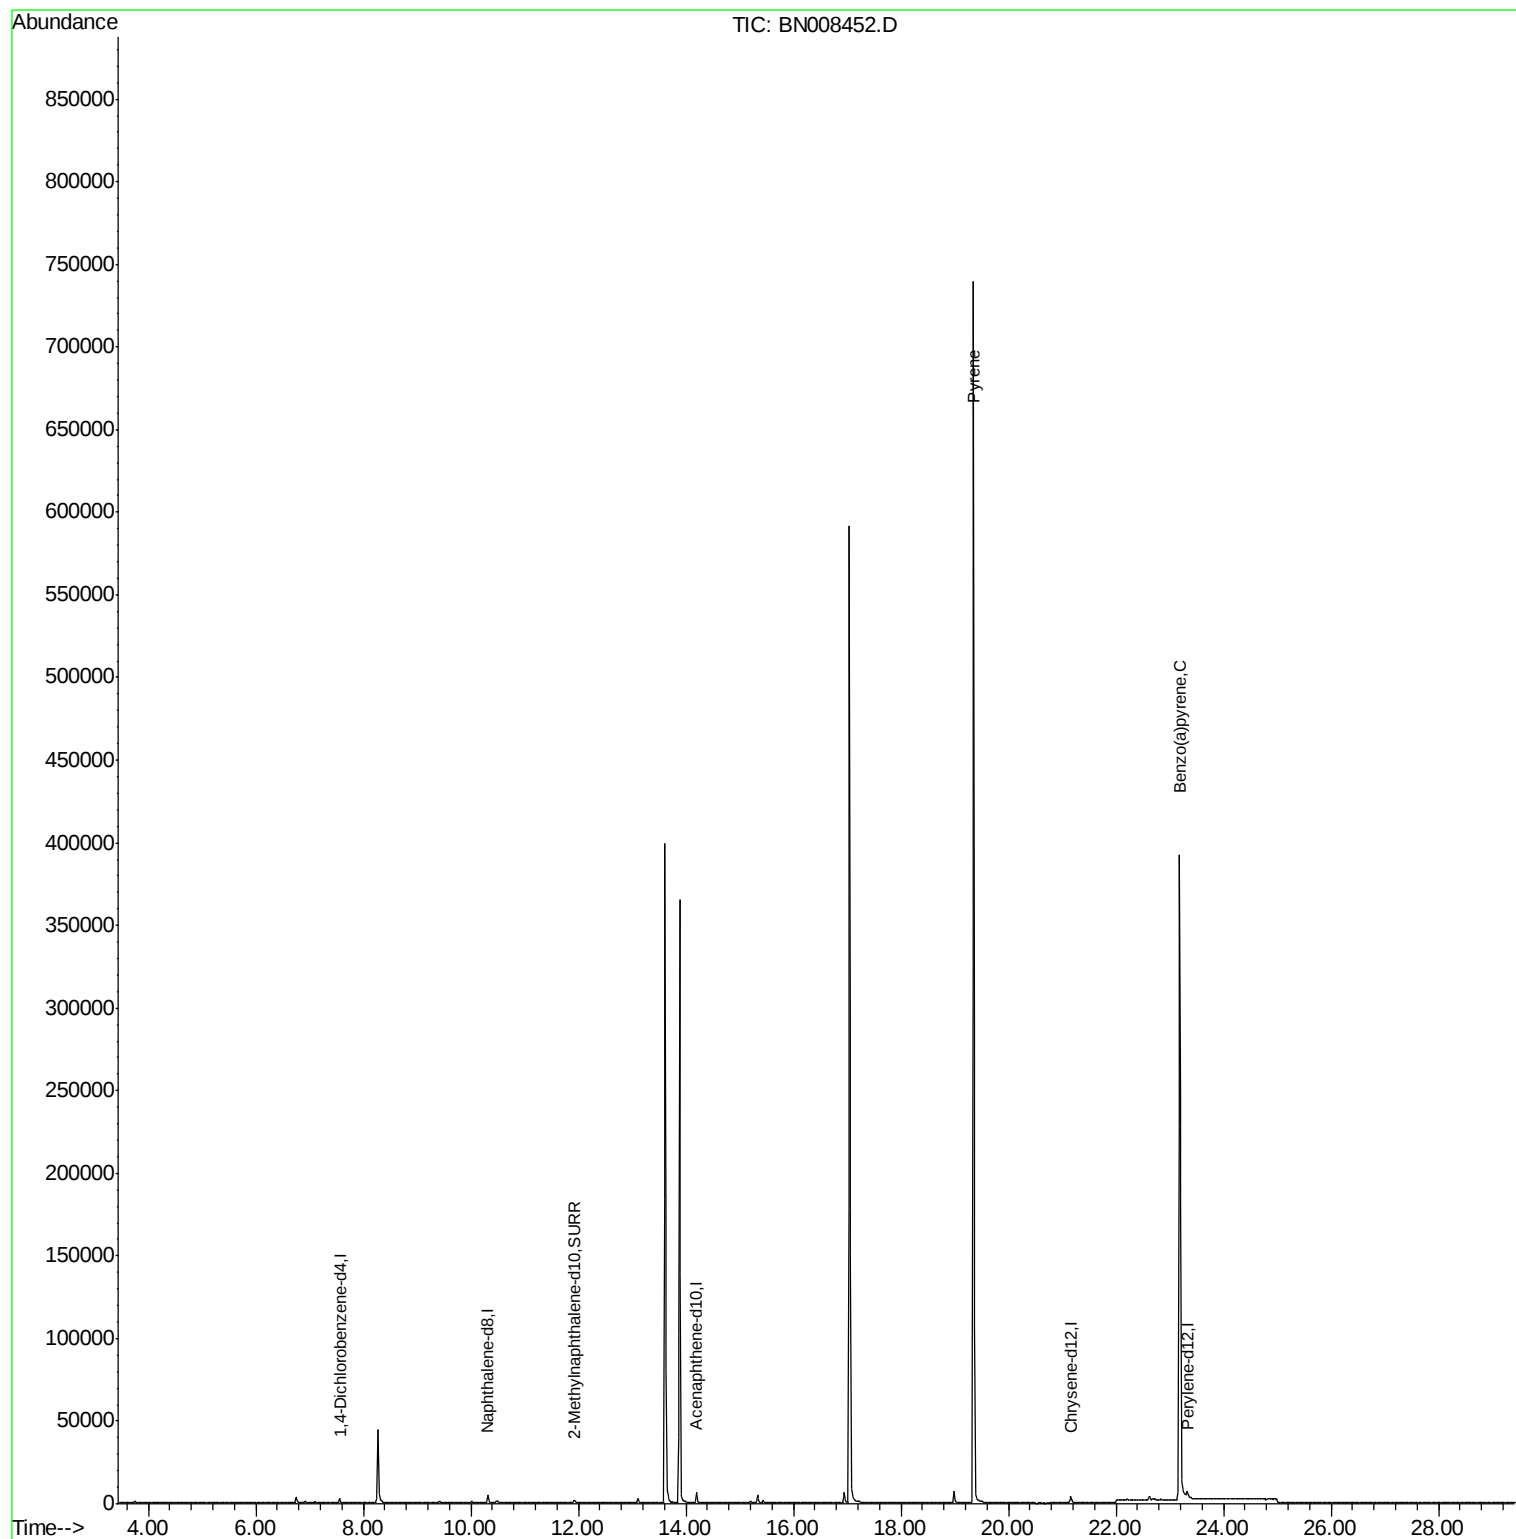

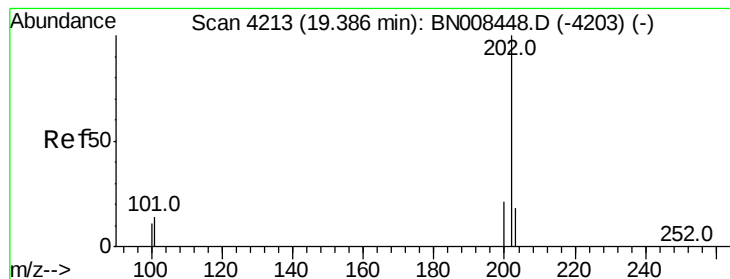

#17

Pvrene

Concen: 0.044 ng/ul

RT: 19.35 min Scan# 4206

Delta R.T. -0.03 min

Lab File: BN008452.D

Acq: 05 Nov 2019 18:13


Instrument :

BNA_N

ClientSampleId :

Tot Ion:202 Resp: 1186




Ion	Ratio	Lower	Upper
202	100		
101	173.7	11.6	17.4#
100	1114.3	9.4	14.0#

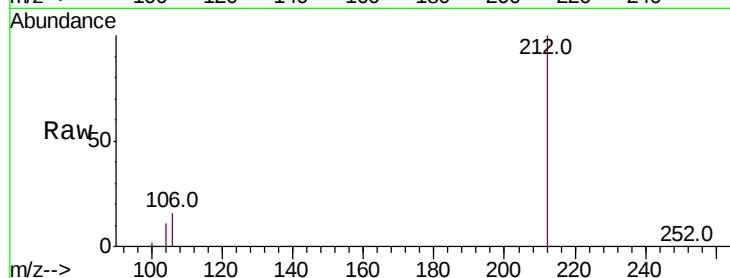

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

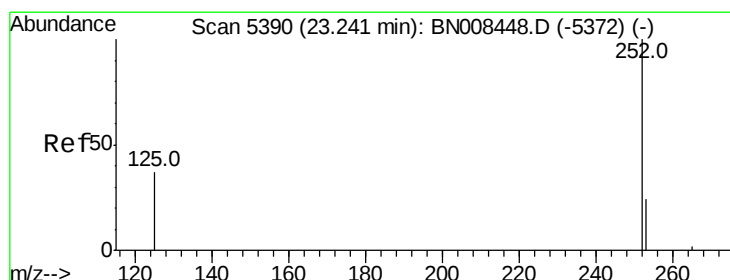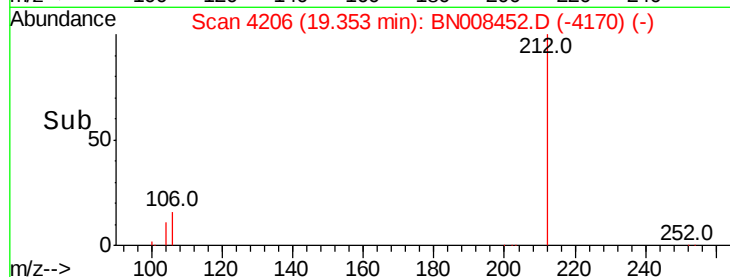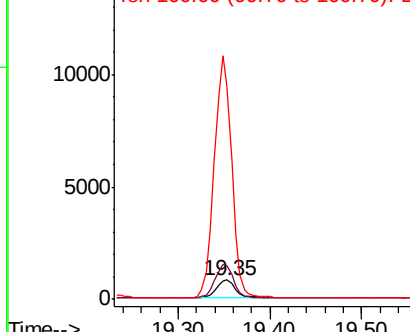

#23

Benzo(a)pyrene

Concen: 0.070 ng/ul

RT: 23.19 min Scan# 5371


Delta R.T. -0.06 min

Lab File: BN008452.D

Acq: 05 Nov 2019 18:13

Tgt Ion:252 Resp: 1794

Ion	Ratio	Lower	Upper
252	100		
253	49.4	27.2	40.8#
125	46.6	37.0	55.6

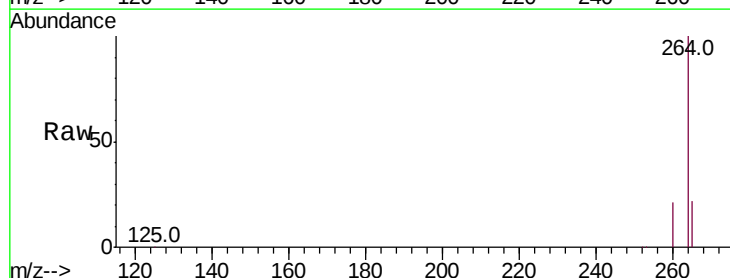

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

