


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110519\
Data File : BN008455.D
Acq On : 05 Nov 2019 20:01
Operator : JU
Sample : K5567-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLNC5

Manual Integrations
APPROVED

mohammad
11/7/2019 2:51:48 PM

Quant Time: Nov 07 11:23:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 10:57:49 2019
Response via : Initial Calibration

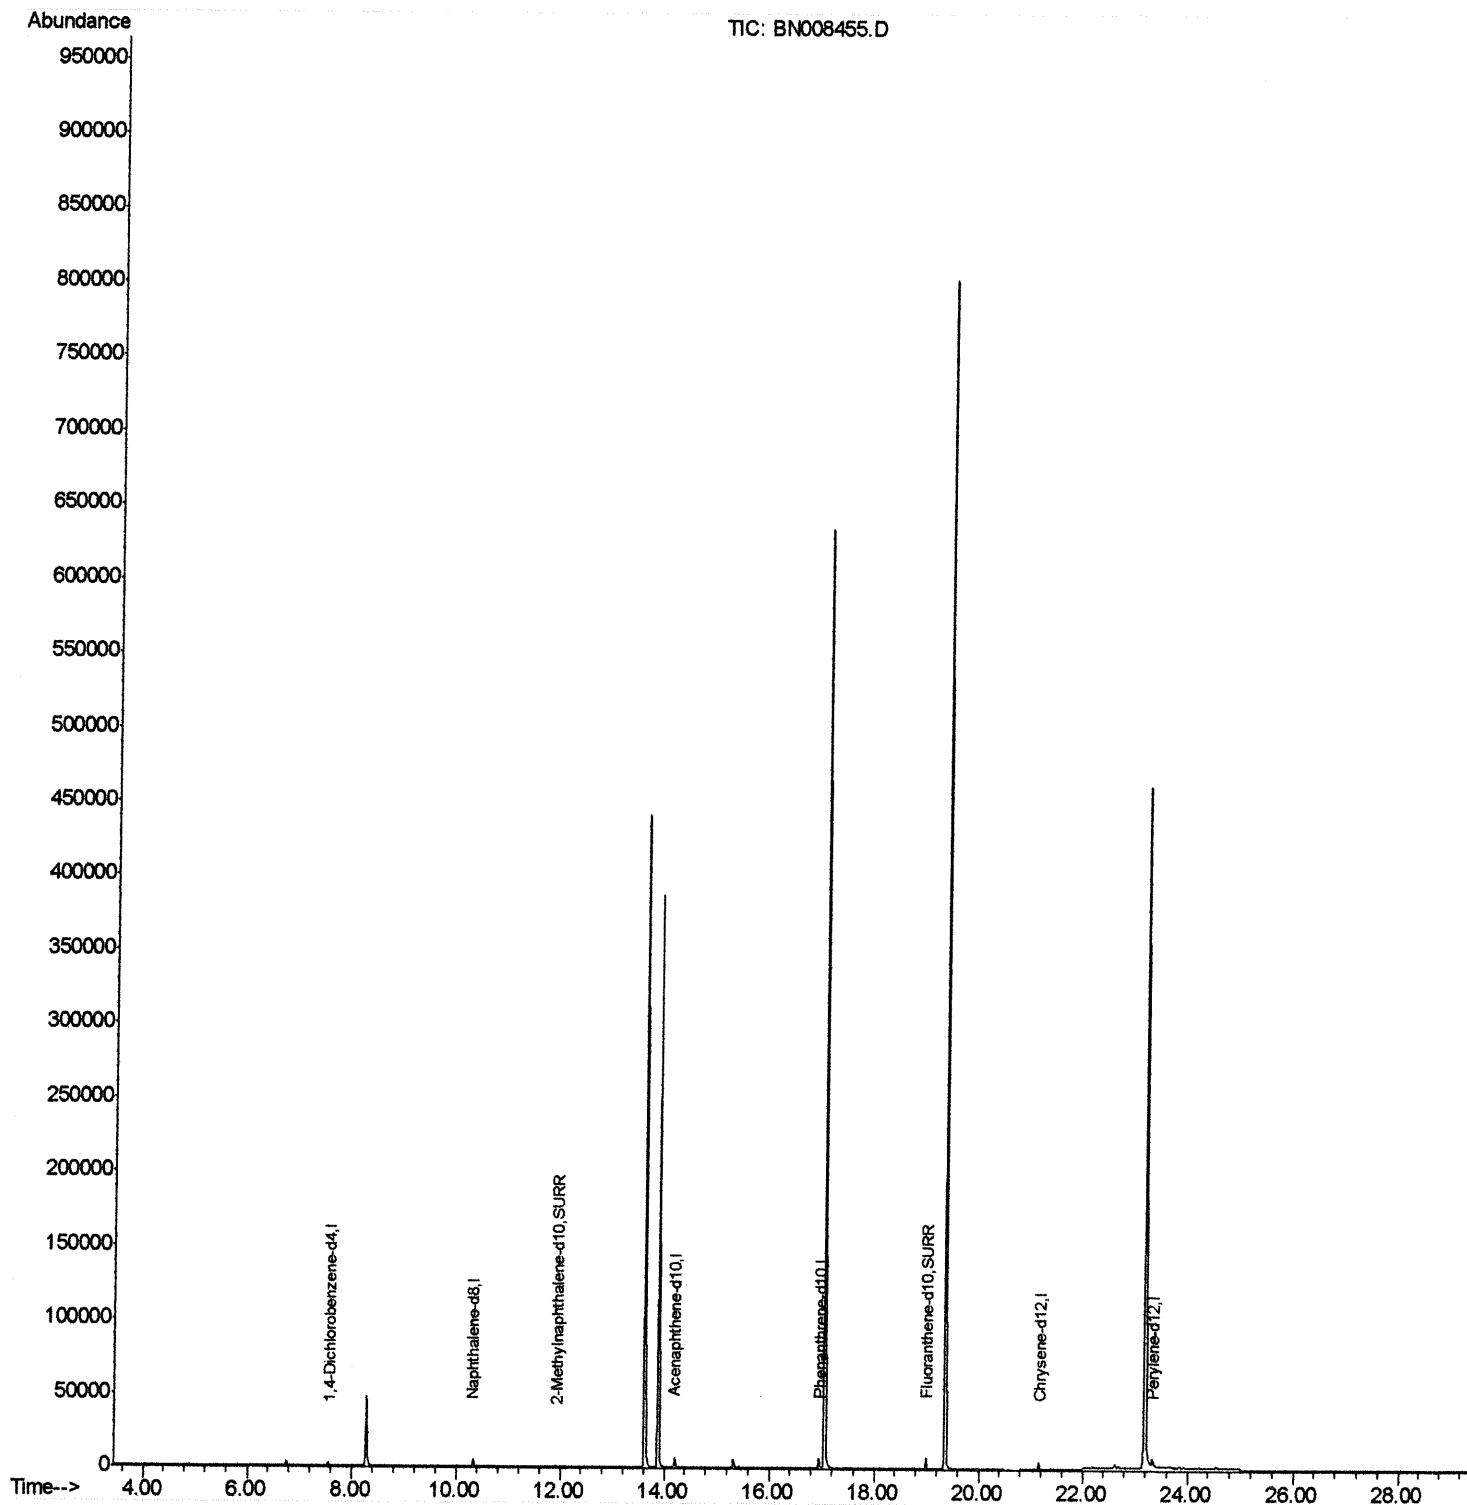

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110519\
 Data File : BN008455.D
 Acq On : 05 Nov 2019 20:01
 Operator : JU
 Sample : K5567-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLNC5

Manual Integrations
 APPROVED

mohammad
 11/7/2019 2:51:48 PM

Quant Time: Nov 07 11:15:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 10:57:49 2019
 Response via : Initial Calibration

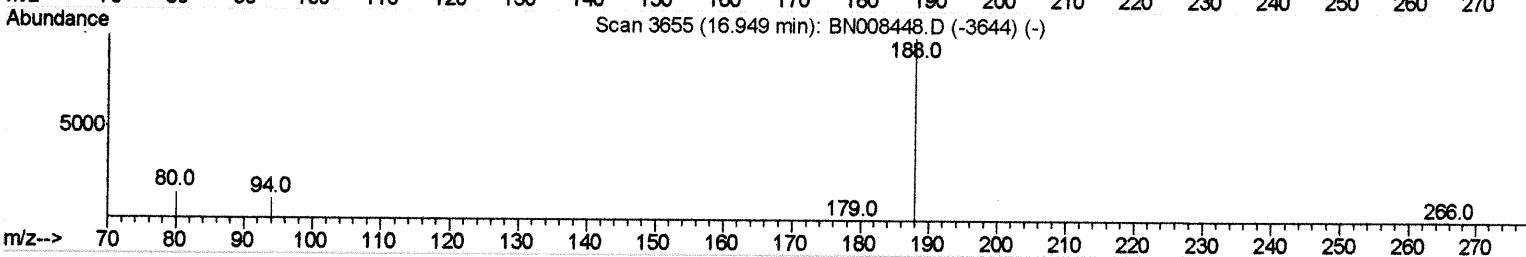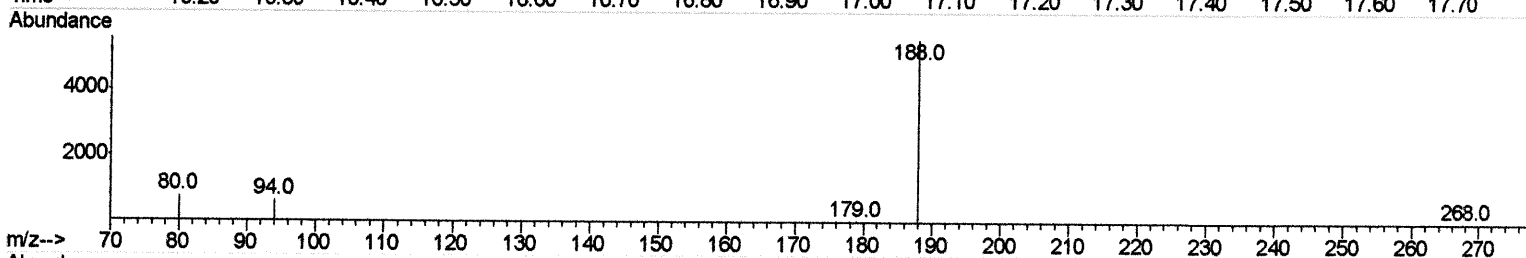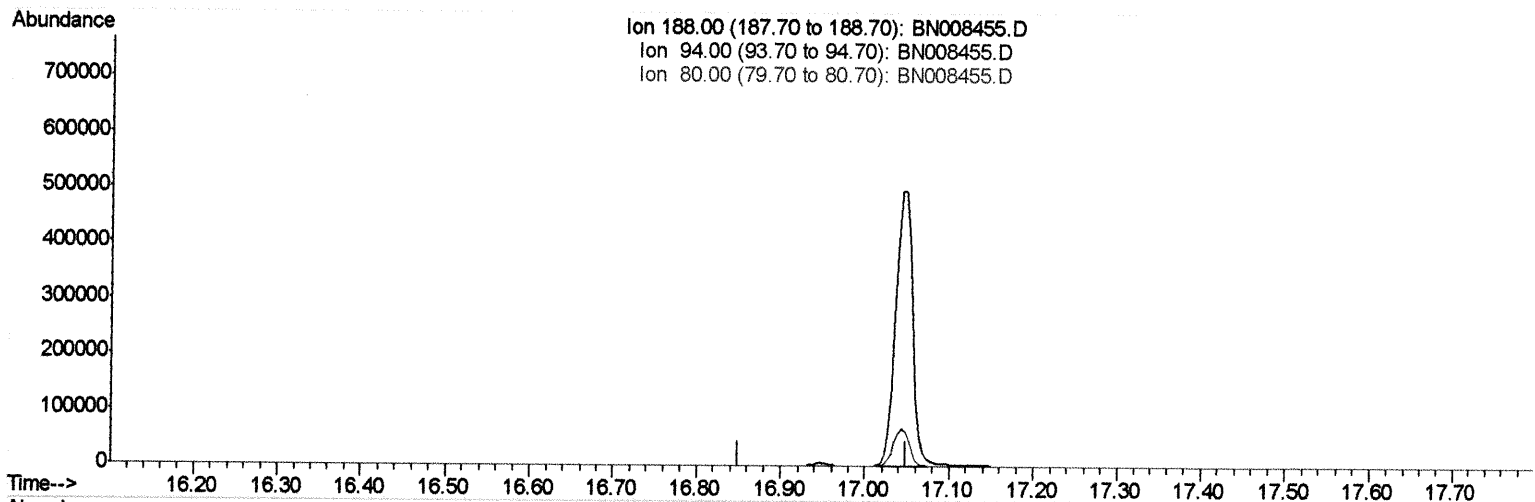

TIC: BN008455.D

(10) Phenanthrene-d10 (I)
 16.949min (-16.949) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	12.40	0.00#
80.00	15.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110519\
 Data File : BN008455.D
 Acq On : 05 Nov 2019 20:01
 Operator : JU
 Sample : K5567-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLNC5

Manual Integrations
 APPROVED

mohammad
 11/7/2019 2:51:48 PM

Quant Time: Nov 07 11:15:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 10:57:49 2019
 Response via : Initial Calibration

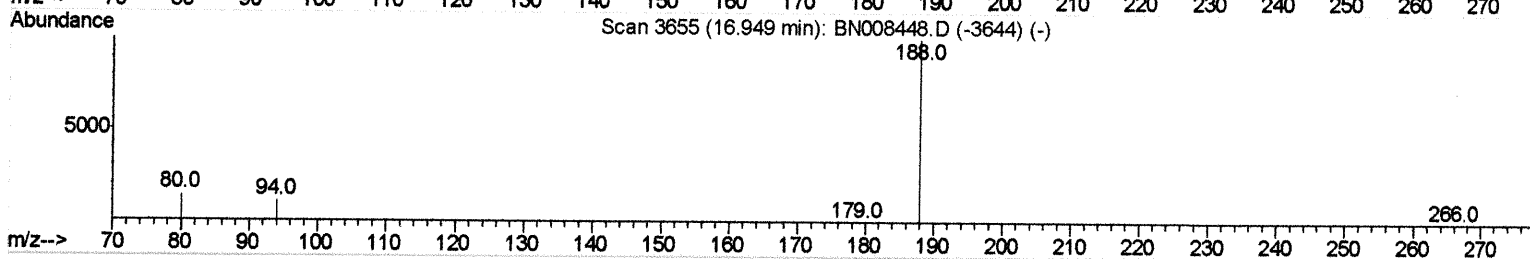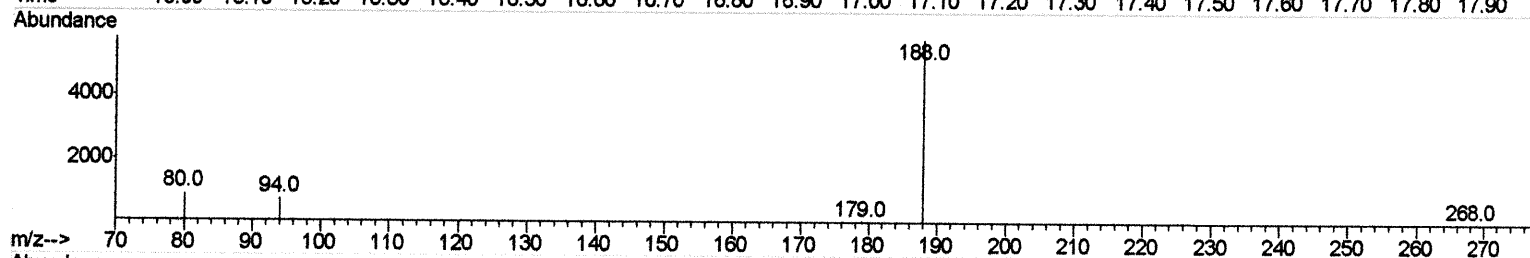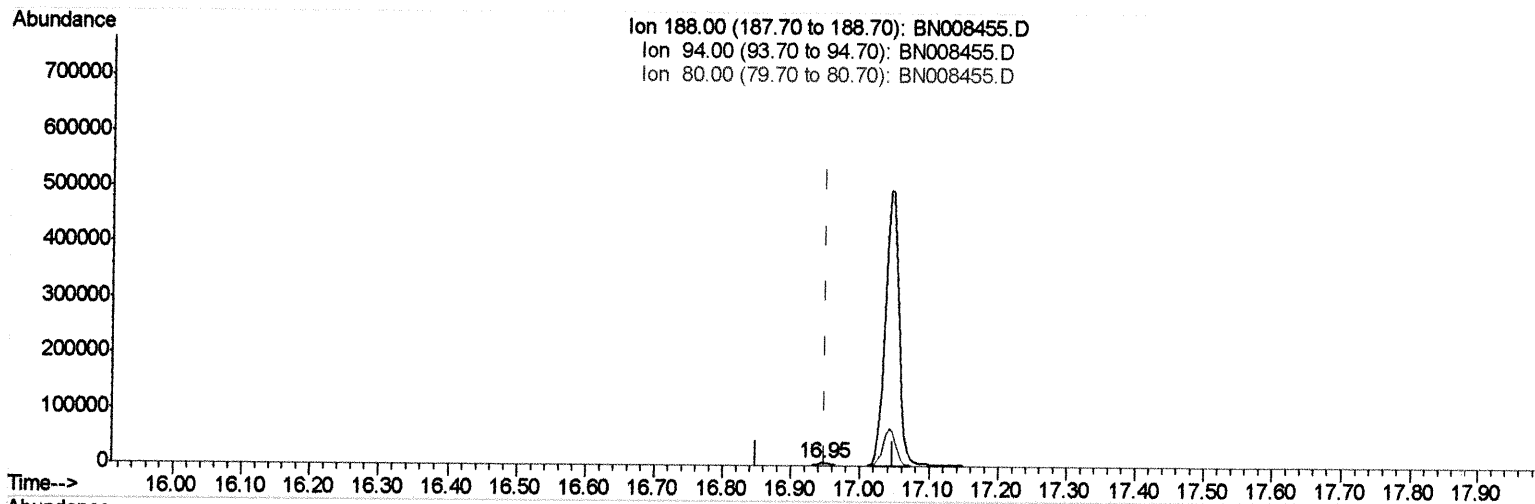

TIC: BN008455.D

(10) Phenanthrene-d10 (I)

16.945min (-0.004) 0.40ng/ul m JU 11/8/19

response 8152

Ion	Exp%	Act%
188.00	100	100
94.00	12.40	12.36
80.00	15.50	15.11
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110519\
Data File : BN008455.D
Acq On : 05 Nov 2019 20:01
Operator : JU
Sample : K5567-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLNC5

Manual Integrations
APPROVED

mohammad
11/7/2019 2:51:48 PM

Quant Time: Nov 07 11:23:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 10:57:49 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	1495	0.40	ng/ul	0.00
2) Naphthalene-d8	10.32	136	6612	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	3938	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.95	188	8152m	0.40	ng/ul	0.00
16) Chrysene-d12	21.16	240	6612	0.40	ng/ul	0.00
20) Perylene-d12	23.32	264	7855	0.40	ng/ul	-0.01

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.93	152	2811	0.27	ng/ul	0.01
14) Fluoranthene-d10	18.99	212	9159	0.38	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

7 JU 11/8/19