


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110519\
Data File : BN008462.D
Acq On : 06 Nov 2019 00:11
Operator : JU
Sample : PB124382BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK82

Manual Integrations
APPROVED

mohammad
11/7/2019 2:52:10 PM

Quant Time: Nov 07 11:33:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 10:57:49 2019
Response via : Initial Calibration

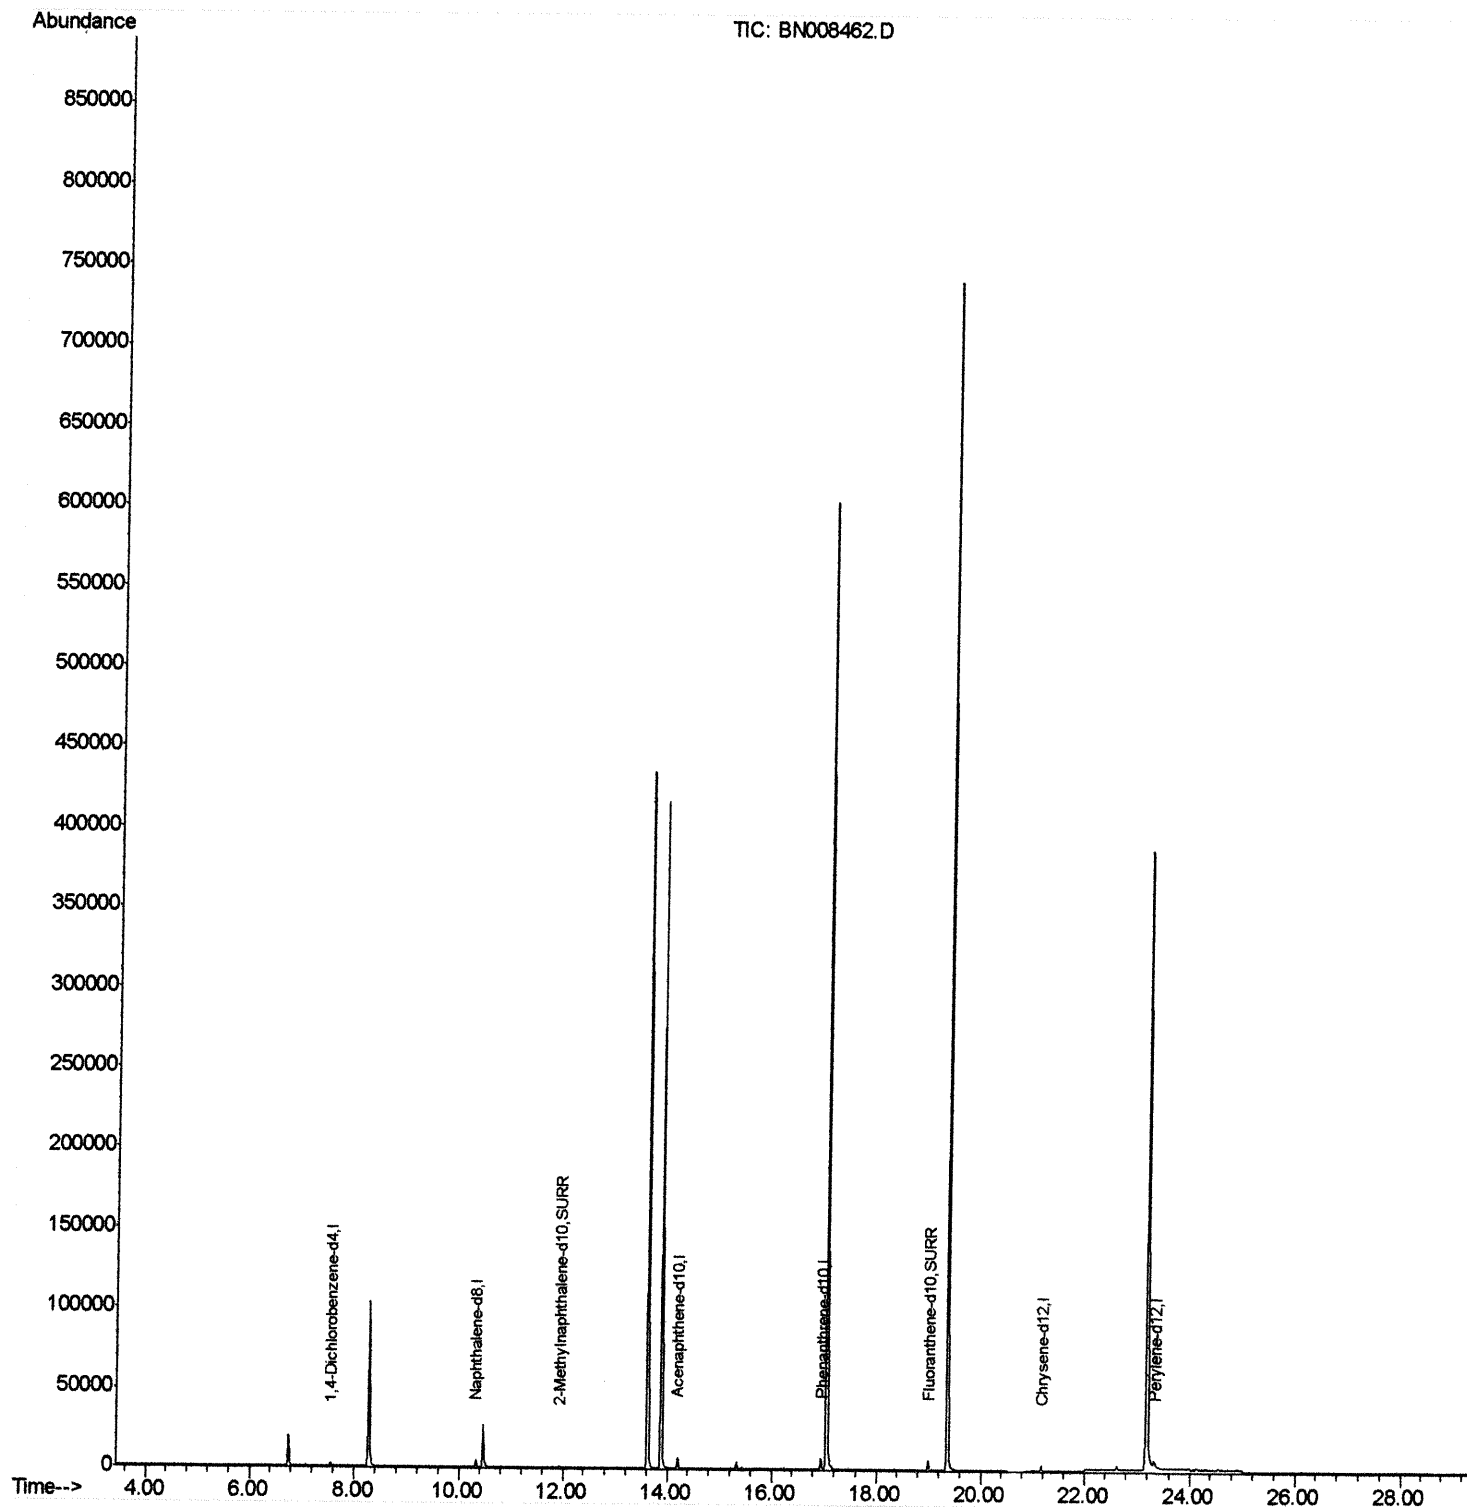

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110519\
 Data File : BN008462.D
 Acq On : 06 Nov 2019 00:11
 Operator : JU
 Sample : PB124382BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK82

Manual Integrations
 APPROVED

mohammad
 11/7/2019 2:52:10 PM

Quant Time: Nov 07 11:15:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 10:57:49 2019
 Response via : Initial Calibration

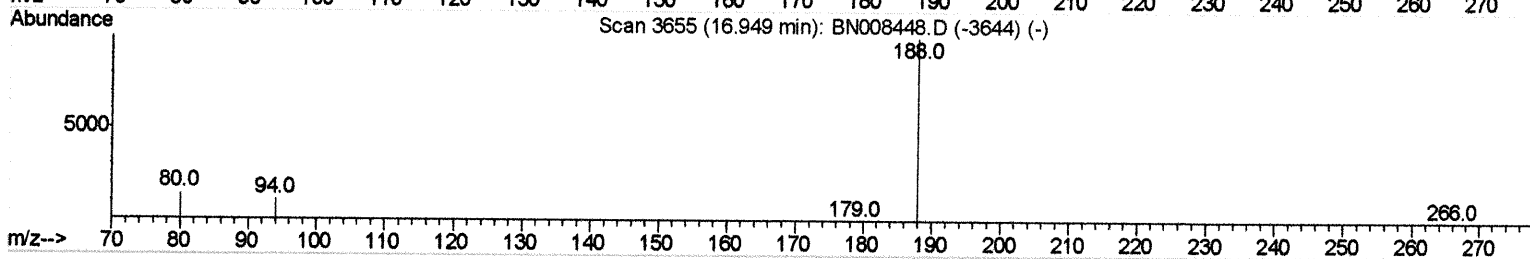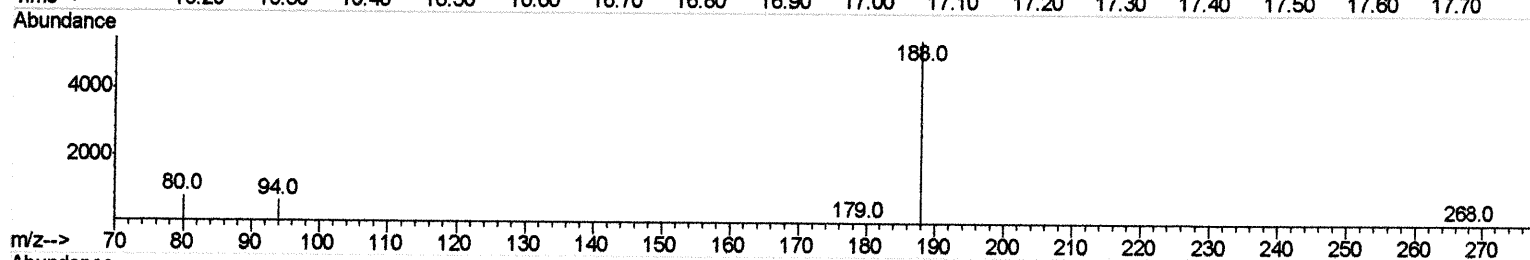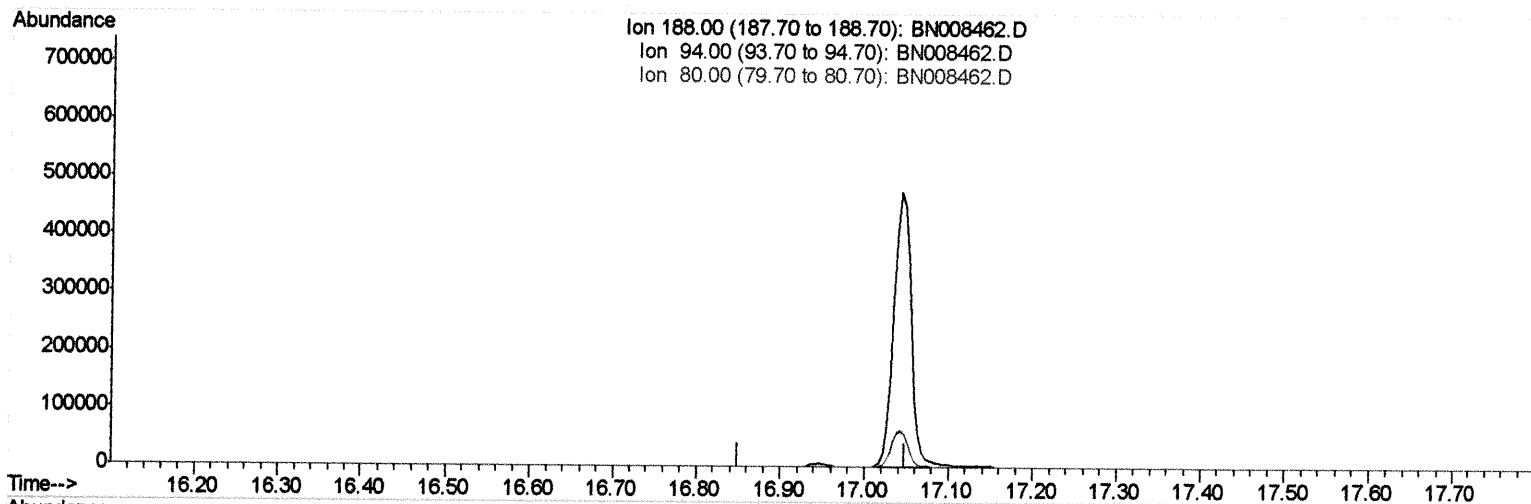

TIC: BN008462.D

(10) Phenanthrene-d10 (I)
 16.949min (-16.949) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	12.40	0.00#
80.00	15.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110519\
 Data File : BN008462.D
 Acq On : 06 Nov 2019 00:11
 Operator : JU
 Sample : PB124382BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK82

Manual Integrations
 APPROVED

mohammad
 11/7/2019 2:52:10 PM

Quant Time: Nov 07 11:15:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 10:57:49 2019
 Response via : Initial Calibration

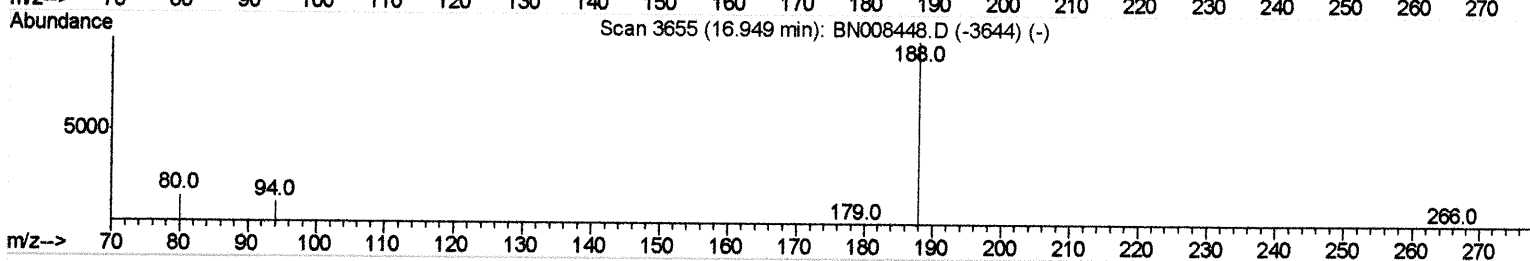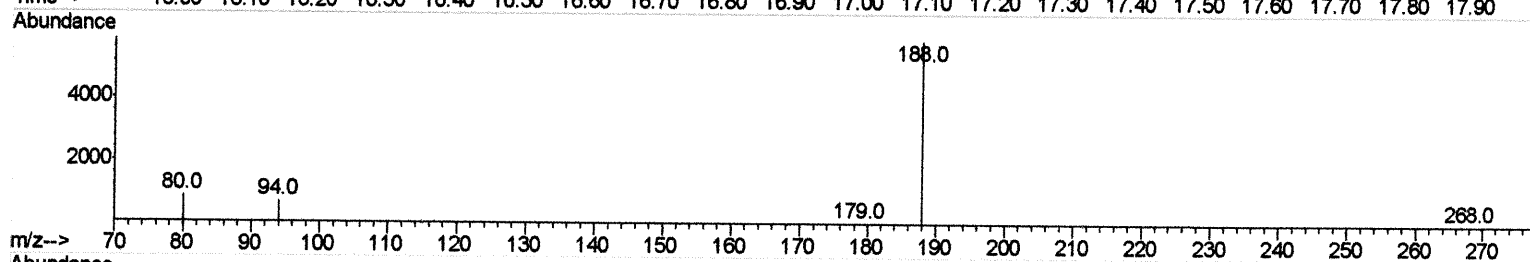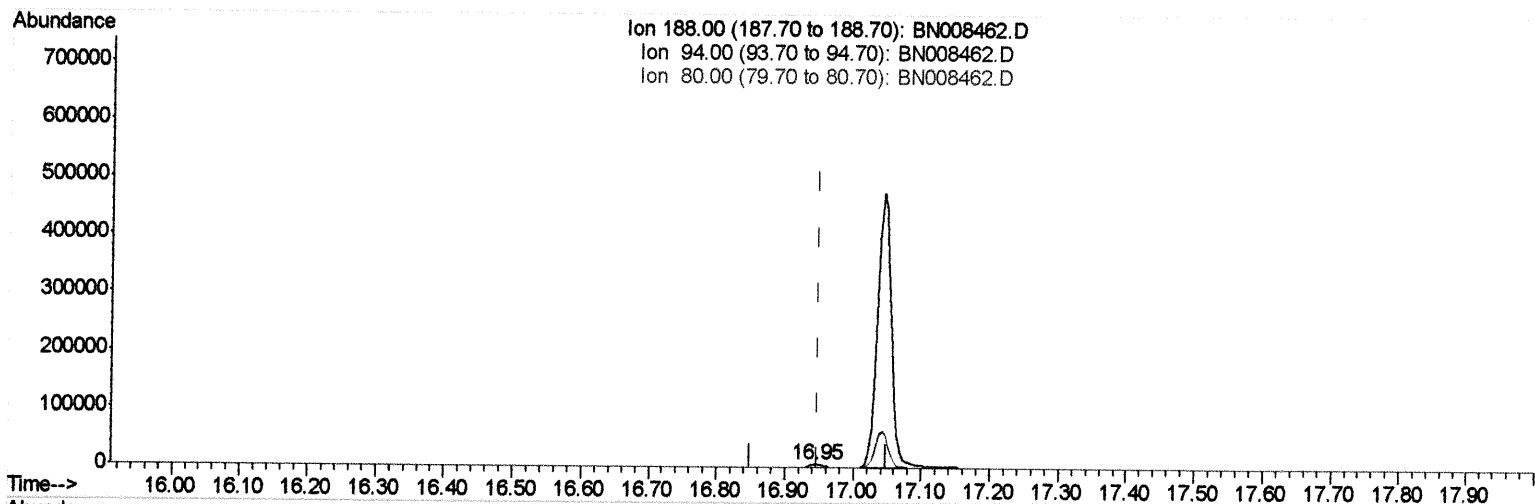

TIC: BN008462.D

(10) Phenanthrene-d10 (I)

16.945min (-0.004) 0.40ng/ul m *JU 11/8/19*

response 8415

Ion	Exp%	Act%
188.00	100	100
94.00	12.40	11.87
80.00	15.50	15.03
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110519\
Data File : BN008462.D
Acq On : 06 Nov 2019 00:11
Operator : JU
Sample : PB124382BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK82

Manual Integrations
APPROVED

mohammad
11/7/2019 2:52:10 PM

Quant Time: Nov 07 11:33:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 10:57:49 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	1527	0.40	ng/ul	0.00
2) Naphthalene-d8	10.32	136	6748	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	4028	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.95	188	8415m>	0.40	ng/ul>	0.00>
16) Chrysene-d12	21.16	240	5885	0.40	ng/ul	0.00
20) Perylene-d12	23.32	264	7576	0.40	ng/ul	-0.01

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.93	152	3125	0.29	ng/ul	0.02
14) Fluoranthene-d10	18.99	212	7772	0.31	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Ju 11/8/19