

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110618\
 Data File : BN003449.D
 Acq On : 07 Nov 2018 01:34
 Operator : MJ/SJ
 Sample : PB114560TB
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB114560TB

Quant Time: Nov 07 10:53:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN102418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 07 08:25:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	99796	20.00	ng	0.00
21) Naphthalene-d8	10.65	136	412458	20.00	ng	0.00
39) Acenaphthene-d10	14.49	164	239958	20.00	ng	0.00
64) Phenanthrene-d10	17.23	188	495090	20.00	ng	0.00
76) Chrysene-d12	21.40	240	410191	20.00	ng	0.00
87) Perylene-d12	23.72	264	430718	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	716309	125.02	ng	0.00
7) Phenol-d6	7.01	99	939298	115.29	ng	0.00
23) Nitrobenzene-d5	9.02	82	524445	72.92	ng	0.00
42) 2,4,6-Tribromophenol	15.97	330	380469	117.75	ng	0.00
45) 2-Fluorobiphenyl	13.11	172	1454485	82.22	ng	0.00
79) Terphenyl-d14	19.85	244	1766499	92.10	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110618\
Data File : BN003449.D
Acq On : 07 Nov 2018 01:34
Operator : MJ/SJ
Sample : PB114560TB
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB114560TB

Quant Time: Nov 07 10:53:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN102418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 07 08:25:32 2018
Response via : Initial Calibration

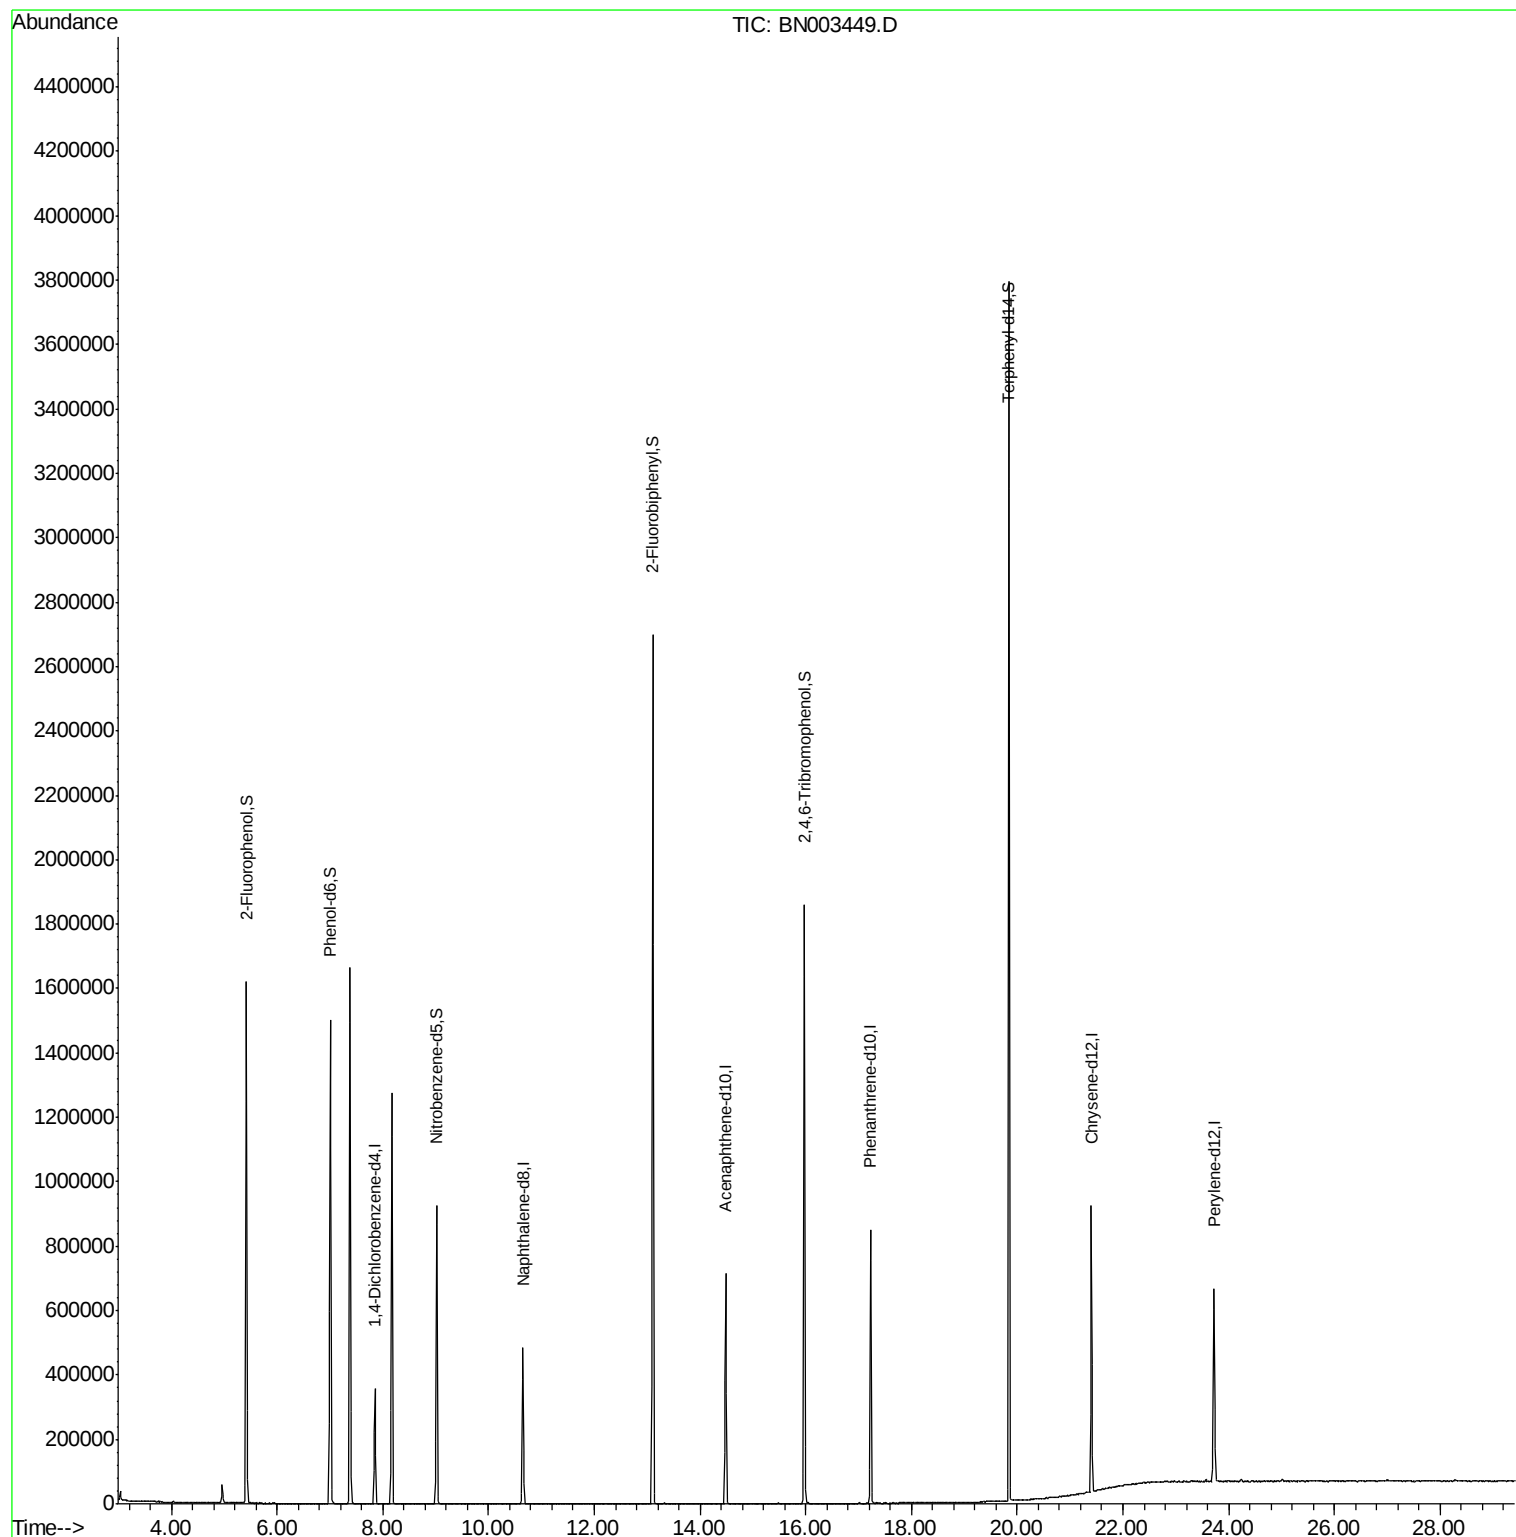

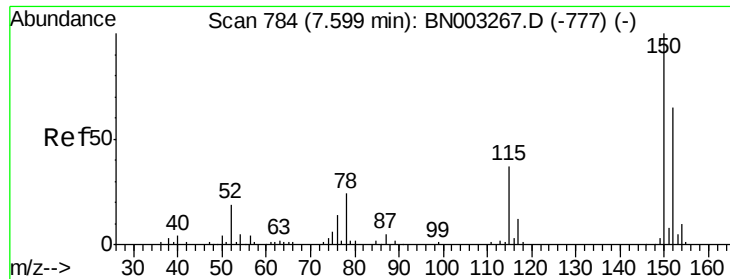


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.85 min Scan# 827
Delta R.T. 0.00 min
Lab File: BN003449.D
Acq: 07 Nov 2018 01:34

Instrument :
BNA_N
ClientSampleId :
PB114560TB

Tgt Ion:152 Resp: 99796
Ion Ratio Lower Upper
152 100
150 155.1 123.8 185.8
115 57.7 45.9 68.9

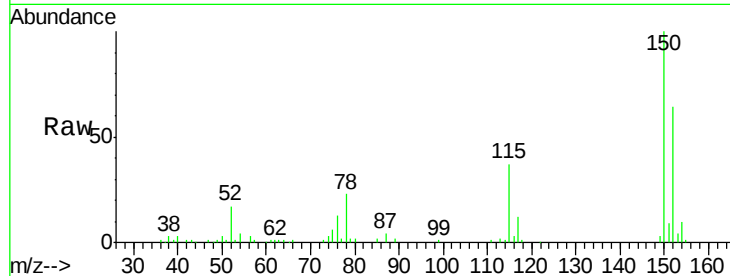


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

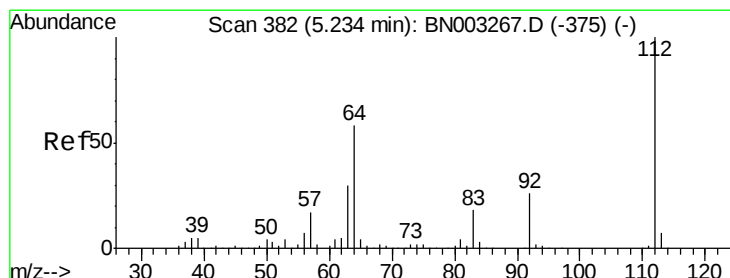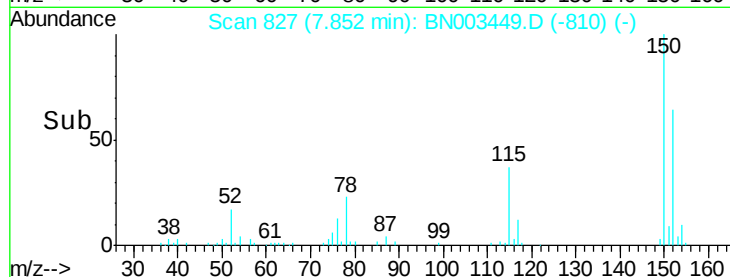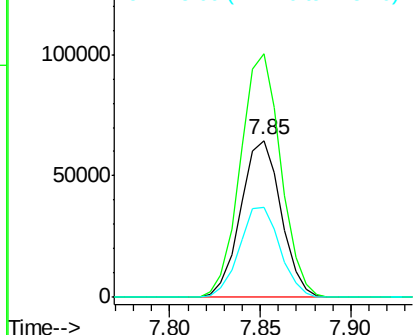



#5


2-Fluorophenol
Concen: 125.018 ng
RT: 5.42 min Scan# 413
Delta R.T. 0.01 min
Lab File: BN003449.D
Acq: 07 Nov 2018 01:34

Tgt Ion:112 Resp: 716309
Ion Ratio Lower Upper
112 100
64 52.8 46.6 69.8
63 26.2 23.8 35.8

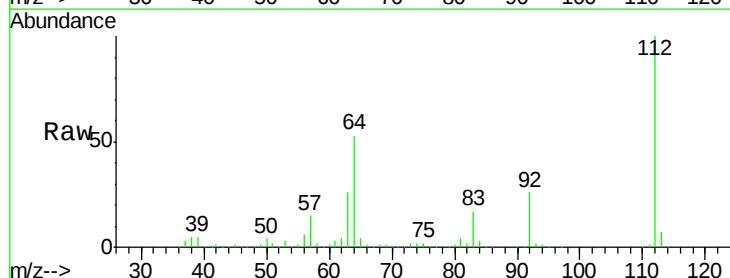

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

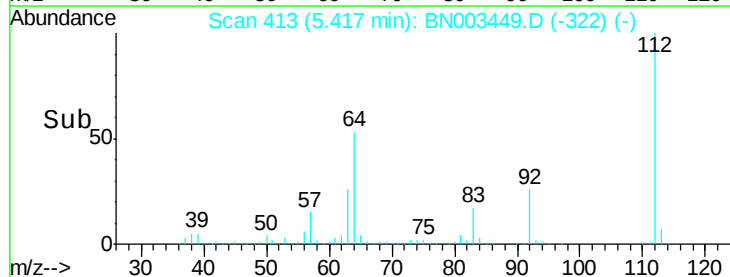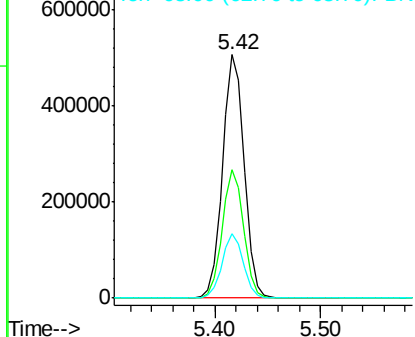

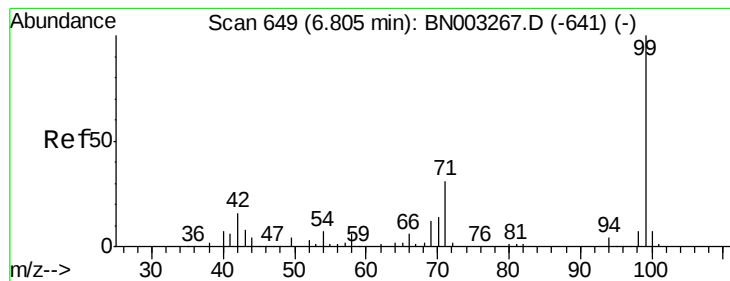

#7

Phenol-d6

Concen: 115.290 ng

RT: 7.01 min Scan# 684

Delta R.T. 0.00 min

Lab File: BN003449.D

Acq: 07 Nov 2018 01:34

Instrument :

BNA_N

ClientSampleId :

PB114560TB


Tgt Ion: 99 Resp: 939298

Ion Ratio Lower Upper

99 100

42 14.5 13.0 19.6




71 29.6 24.5 36.7

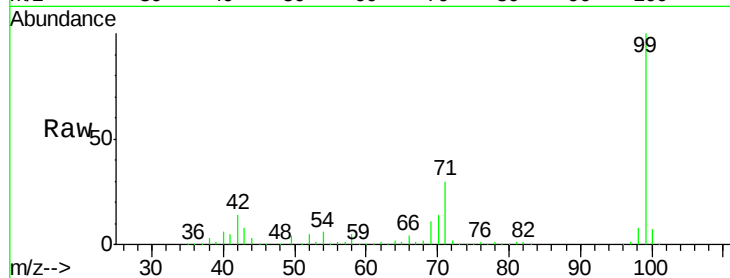

Abundance Ion 99.00 (98.70 to 99.70): BN003267.D (-641) (-)

Ion 42.00 (41.70 to 42.70): BN003267.D (-641) (-)

Ion 71.00 (70.70 to 71.70): BN003267.D (-641) (-)

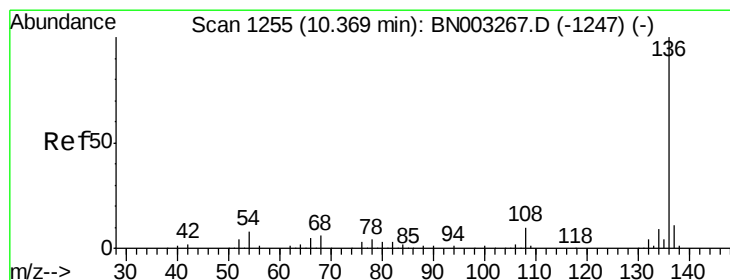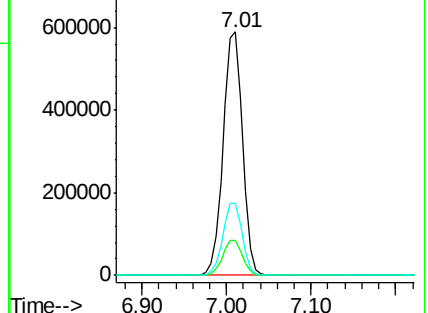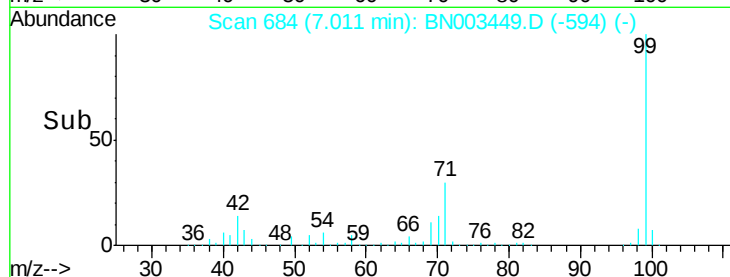

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.65 min Scan# 1302

Delta R.T. -0.01 min

Lab File: BN003449.D

Acq: 07 Nov 2018 01:34

Tgt Ion: 136 Resp: 412458


Ion Ratio Lower Upper

136 100

137 11.2 8.7 13.1

54 7.3 6.6 10.0

68 6.3 4.6 7.0


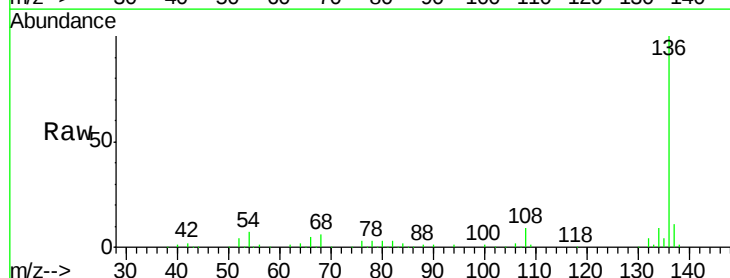



Abundance Ion 136.00 (135.70 to 136.70): BN003267.D (-1247) (-)

Ion 137.00 (136.70 to 137.70): BN003267.D (-1247) (-)

Ion 54.00 (53.70 to 54.70): BN003267.D (-1247) (-)

Ion 68.00 (67.70 to 68.70): BN003267.D (-1247) (-)



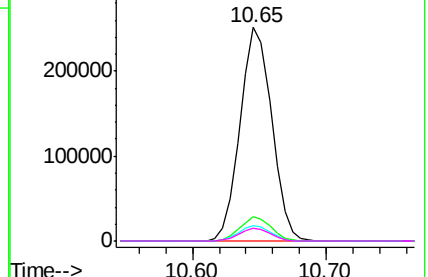
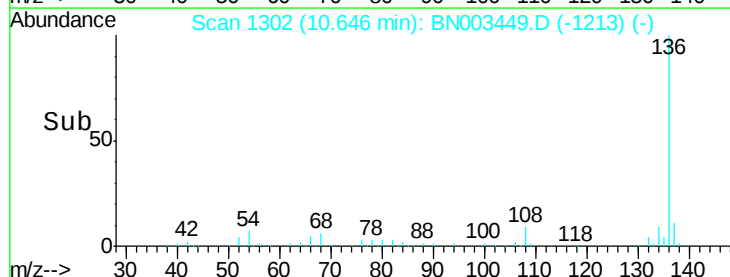


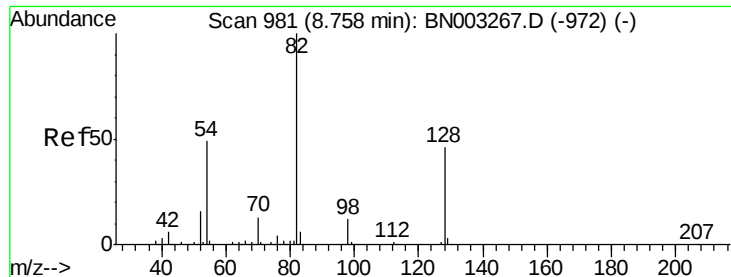

#23
 Nitrobenzene-d5
 Concen: 72.920 ng
 RT: 9.02 min Scan# 1025
 Delta R.T. -0.01 min
 Lab File: BN003449.D
 Acq: 07 Nov 2018 01:34




Instrument :
 BNA_N
 ClientSampleId :
 PB114560TB


Tgt Ion: 82 Resp: 524445
 Ion Ratio Lower Upper
 82 100
 128 49.7 37.1 55.7
 54 45.5 39.4 59.2

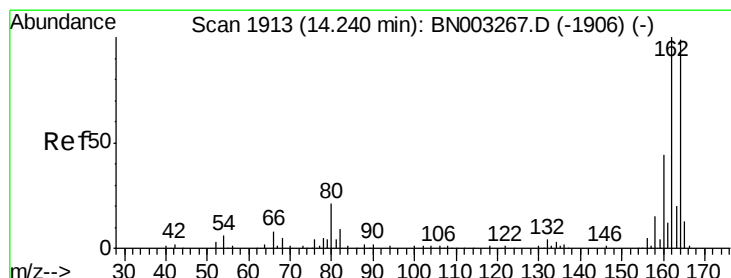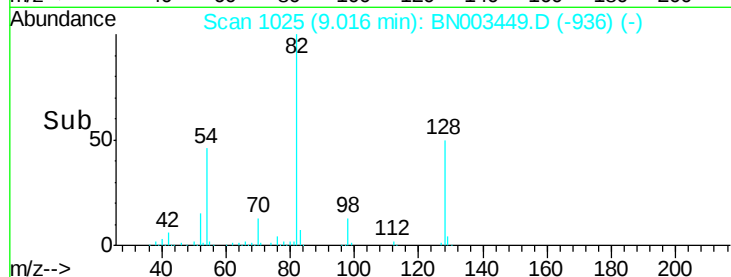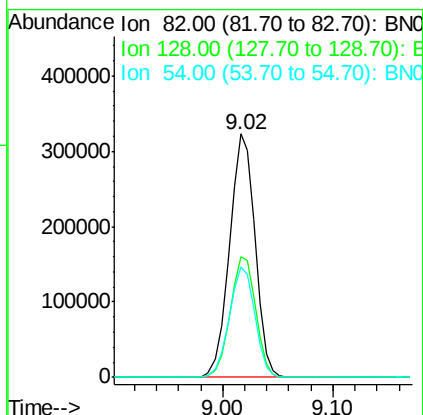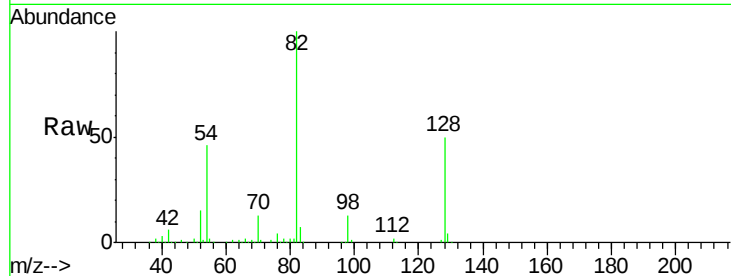

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.49 min Scan# 1955
 Delta R.T. 0.00 min
 Lab File: BN003449.D
 Acq: 07 Nov 2018 01:34

Tgt Ion: 164 Resp: 239958
 Ion Ratio Lower Upper
 164 100
 162 102.4 80.8 121.2
 160 45.3 35.5 53.3

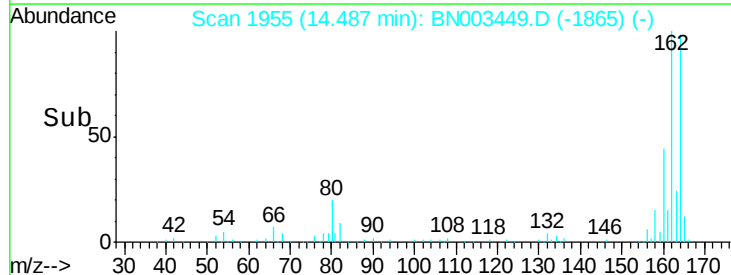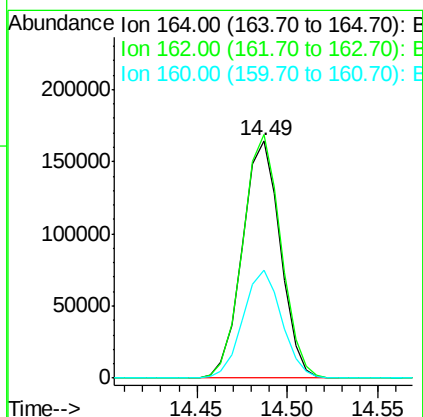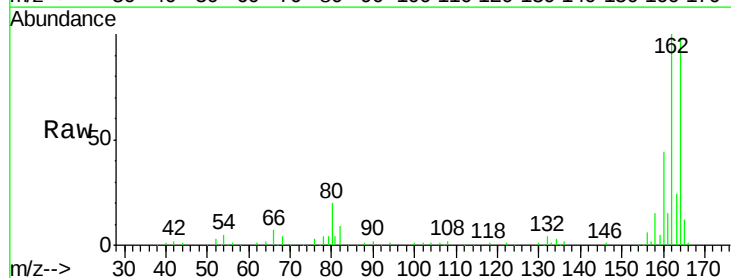


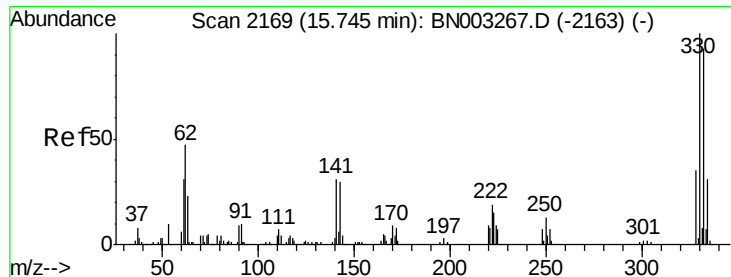




#42
 2,4,6-Tribromophenol
 Concen: 117.752 ng
 RT: 15.97 min Scan# 2208
 Delta R.T. -0.01 min
 Lab File: BN003449.D
 Acq: 07 Nov 2018 01:34

Instrument :
 BNA_N
 ClientSampleId :
 PB114560TB

Tgt Ion:330 Resp: 380469
 Ion Ratio Lower Upper
 330 100
 332 96.2 76.6 114.8
 141 27.3 24.5 36.7

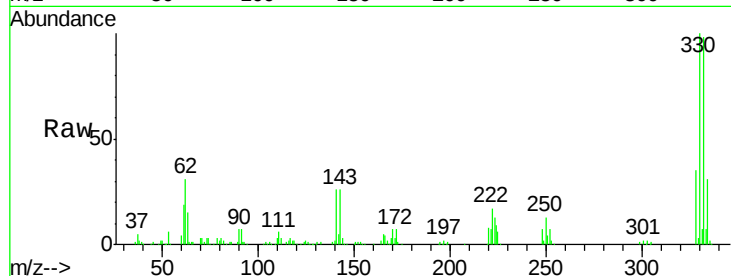


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

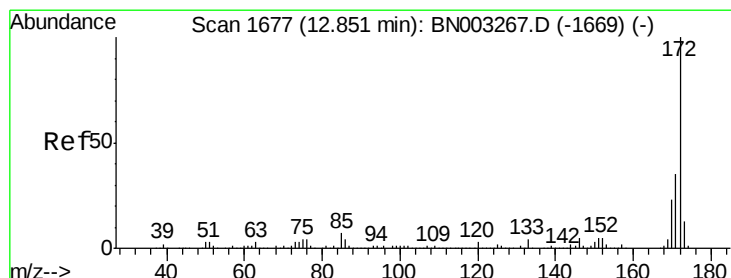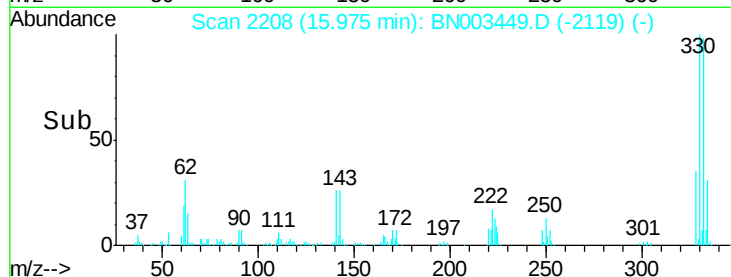
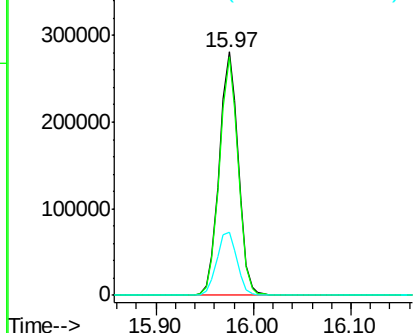



#45
 2-Fluorobiphenyl
 Concen: 82.219 ng
 RT: 13.11 min Scan# 1721
 Delta R.T. 0.00 min
 Lab File: BN003449.D
 Acq: 07 Nov 2018 01:34

Tgt Ion:172 Resp: 1454485
 Ion Ratio Lower Upper
 172 100
 171 35.5 28.2 42.4
 170 23.2 18.4 27.6

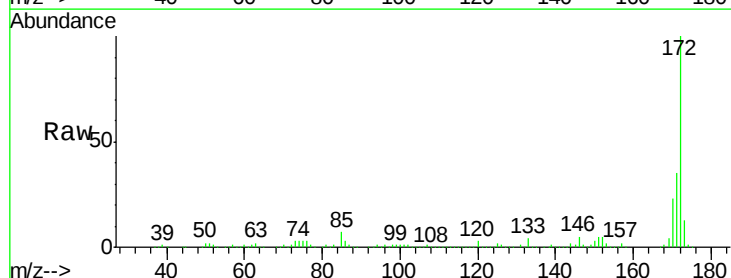

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

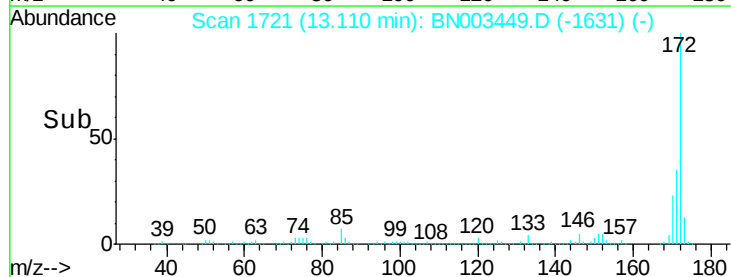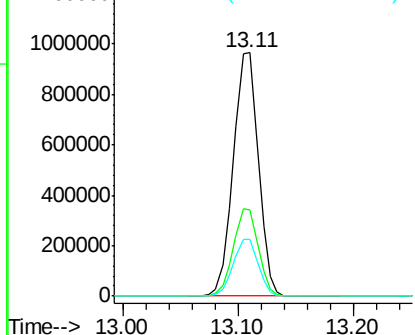


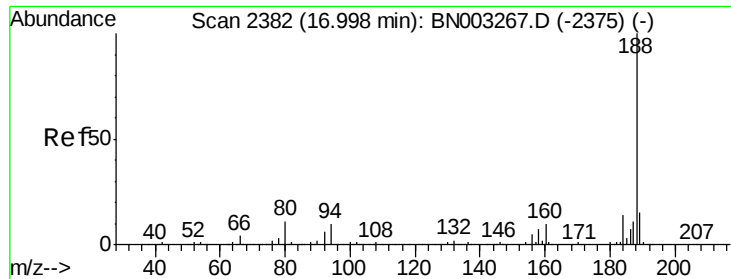




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.23 min Scan# 2421
Delta R.T. -0.01 min
Lab File: BN003449.D
Acq: 07 Nov 2018 01:34

Instrument :
BNA_N
ClientSampleId :
PB114560TB

Tgt Ion:188 Resp: 495090
Ion Ratio Lower Upper
188 100
94 9.7 8.1 12.1
80 10.5 8.6 13.0

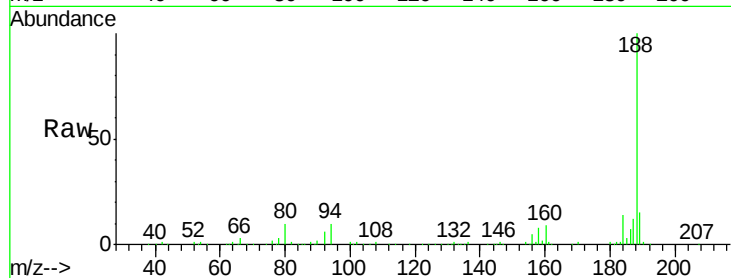


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BNC
Ion 80.00 (79.70 to 80.70): BNC

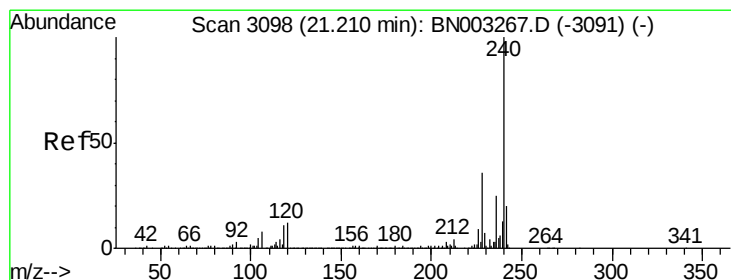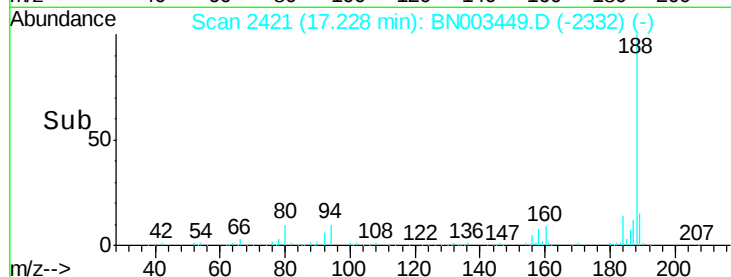
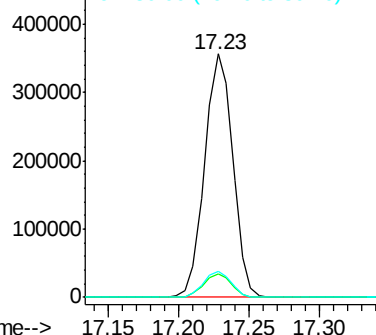



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.40 min Scan# 3131
Delta R.T. -0.01 min
Lab File: BN003449.D
Acq: 07 Nov 2018 01:34

Tgt Ion:240 Resp: 410191
Ion Ratio Lower Upper
240 100
120 11.5 9.4 14.0
236 25.0 20.3 30.5

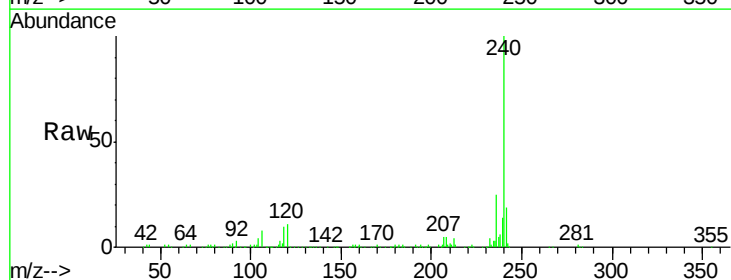

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

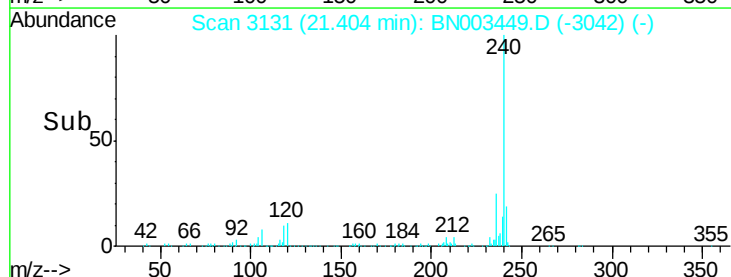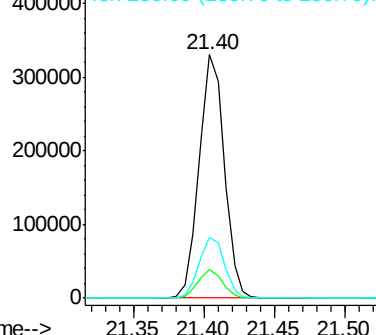

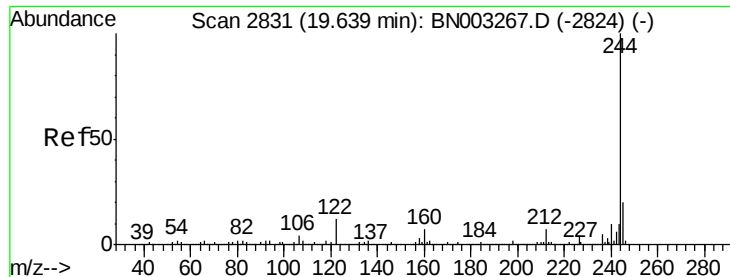

#79

Terphenyl-d14

Concen: 92.097 ng

RT: 19.85 min Scan# 2866

Delta R.T. -0.01 min

Lab File: BN003449.D

Acq: 07 Nov 2018 01:34

Instrument :

BNA_N

ClientSampleId :

PB114560TB


Tgt Ion:244 Resp: 1766499

Ion Ratio Lower Upper

244 100

212 6.7 5.4 8.0




122 10.8 9.4 14.2

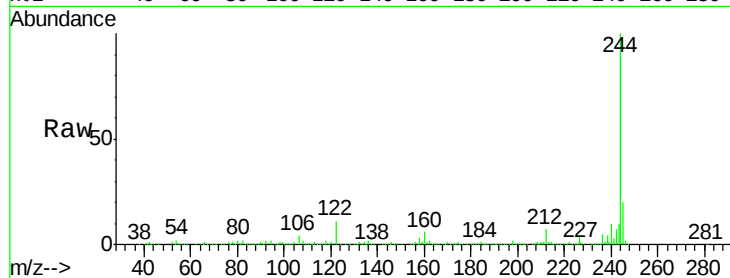

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

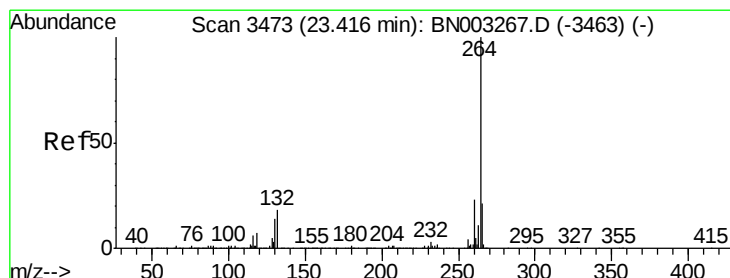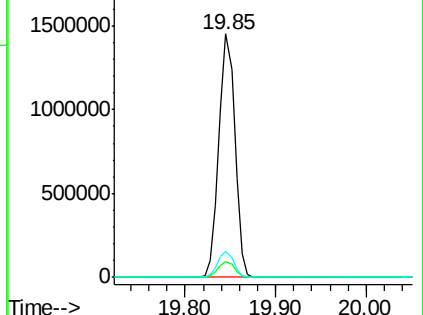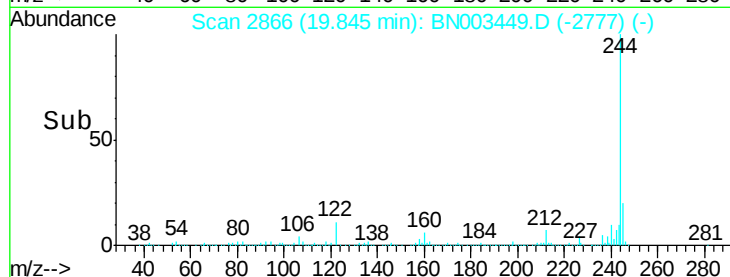

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.72 min Scan# 3525

Delta R.T. -0.01 min

Lab File: BN003449.D

Acq: 07 Nov 2018 01:34


Tgt Ion:264 Resp: 430718

Ion Ratio Lower Upper

264 100

260 23.8 18.5 27.7

265 21.3 16.6 25.0

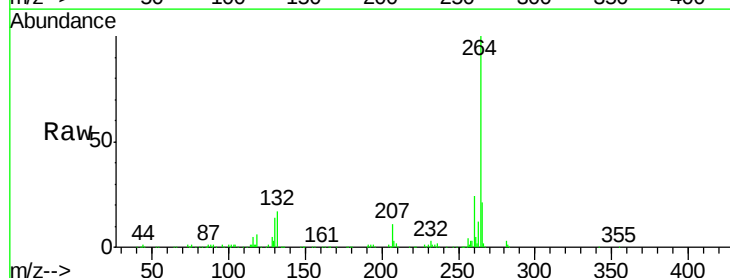

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

