


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110618\
 Data File : BN003436.D
 Acq On : 06 Nov 2018 16:53
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN102418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 07 08:25:32 2018

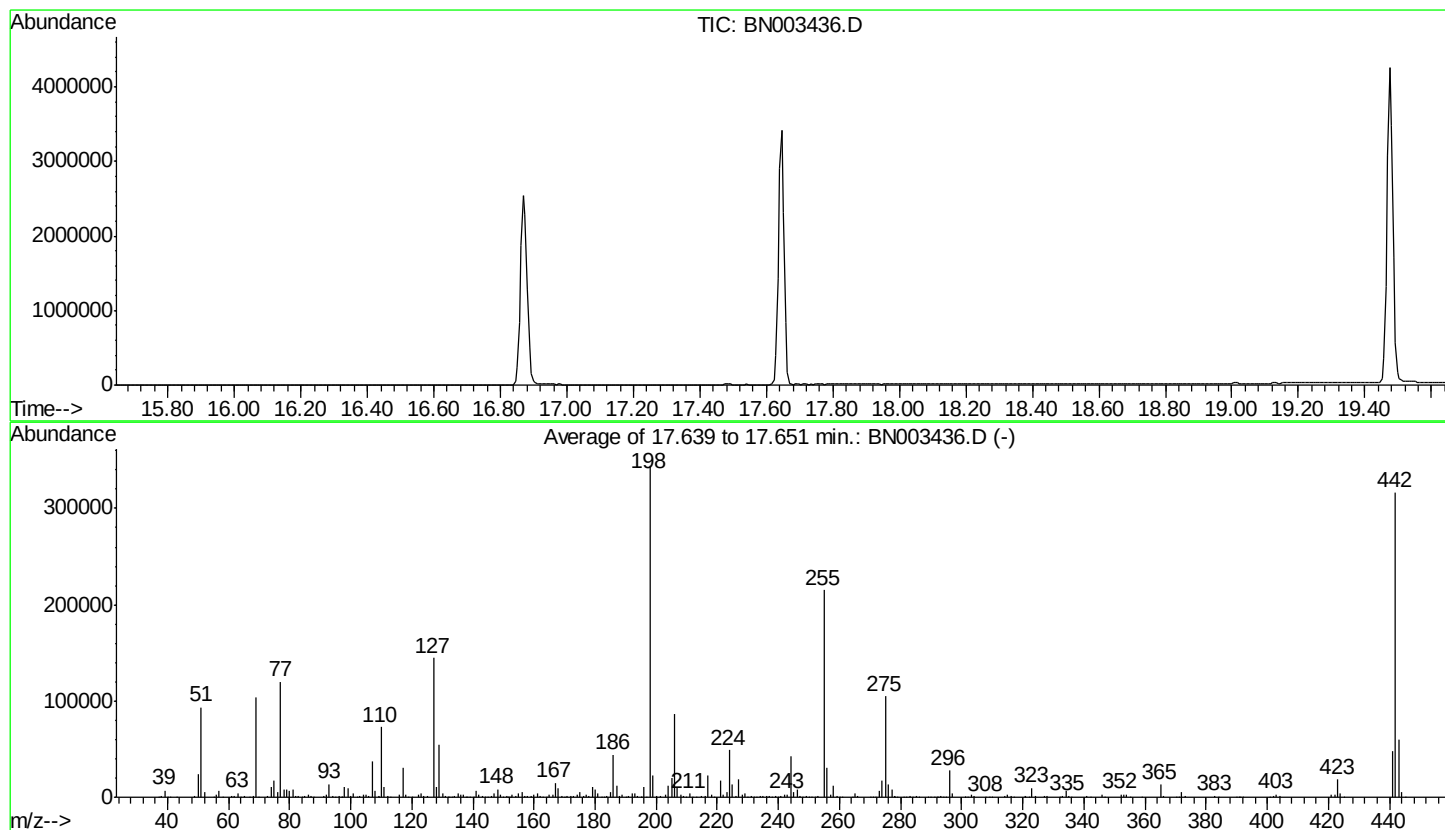

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.2	93722	PASS
68	69	0.00	2	1.8	1875	PASS
69	198	0.00	100	30.0	103458	PASS
70	69	0.00	2	0.6	645	PASS
127	198	10	80	42.1	144925	PASS
197	198	0.00	2	0.2	647	PASS
198	198	100	100	100.0	344512	PASS
199	198	5	9	6.7	23074	PASS
275	198	10	60	30.4	104821	PASS
365	198	1	100	3.7	12869	PASS
441	198	0.01	100	13.8	47629	PASS
442	198	50	100	91.7	315925	PASS
443	442	15	24	18.9	59813	PASS