

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
 Data File : BN008467.D
 Acq On : 06 Nov 2019 15:23
 Operator : JU
 Sample : K5656-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Nov 07 12:25:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 12:16:36 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	1131	0.40	ng/ul	0.00
2) Naphthalene-d8	10.32	136	4905	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	2934	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.95
16) Chrysene-d12	21.16	240	4643	0.40	ng/ul	0.00
20) Perylene-d12	23.33	264	4047	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.93	152	2133	0.28	ng/ul	0.02
14) Fluoranthene-d10	18.99	212	6587	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.35	202	1079	0.048	ng/ul#	1
23) Benzo(a)pyrene	23.19	252	1627	0.107	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
Data File : BN008467.D
Acq On : 06 Nov 2019 15:23
Operator : JU
Sample : K5656-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Nov 07 12:25:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 12:16:36 2019
Response via : Initial Calibration

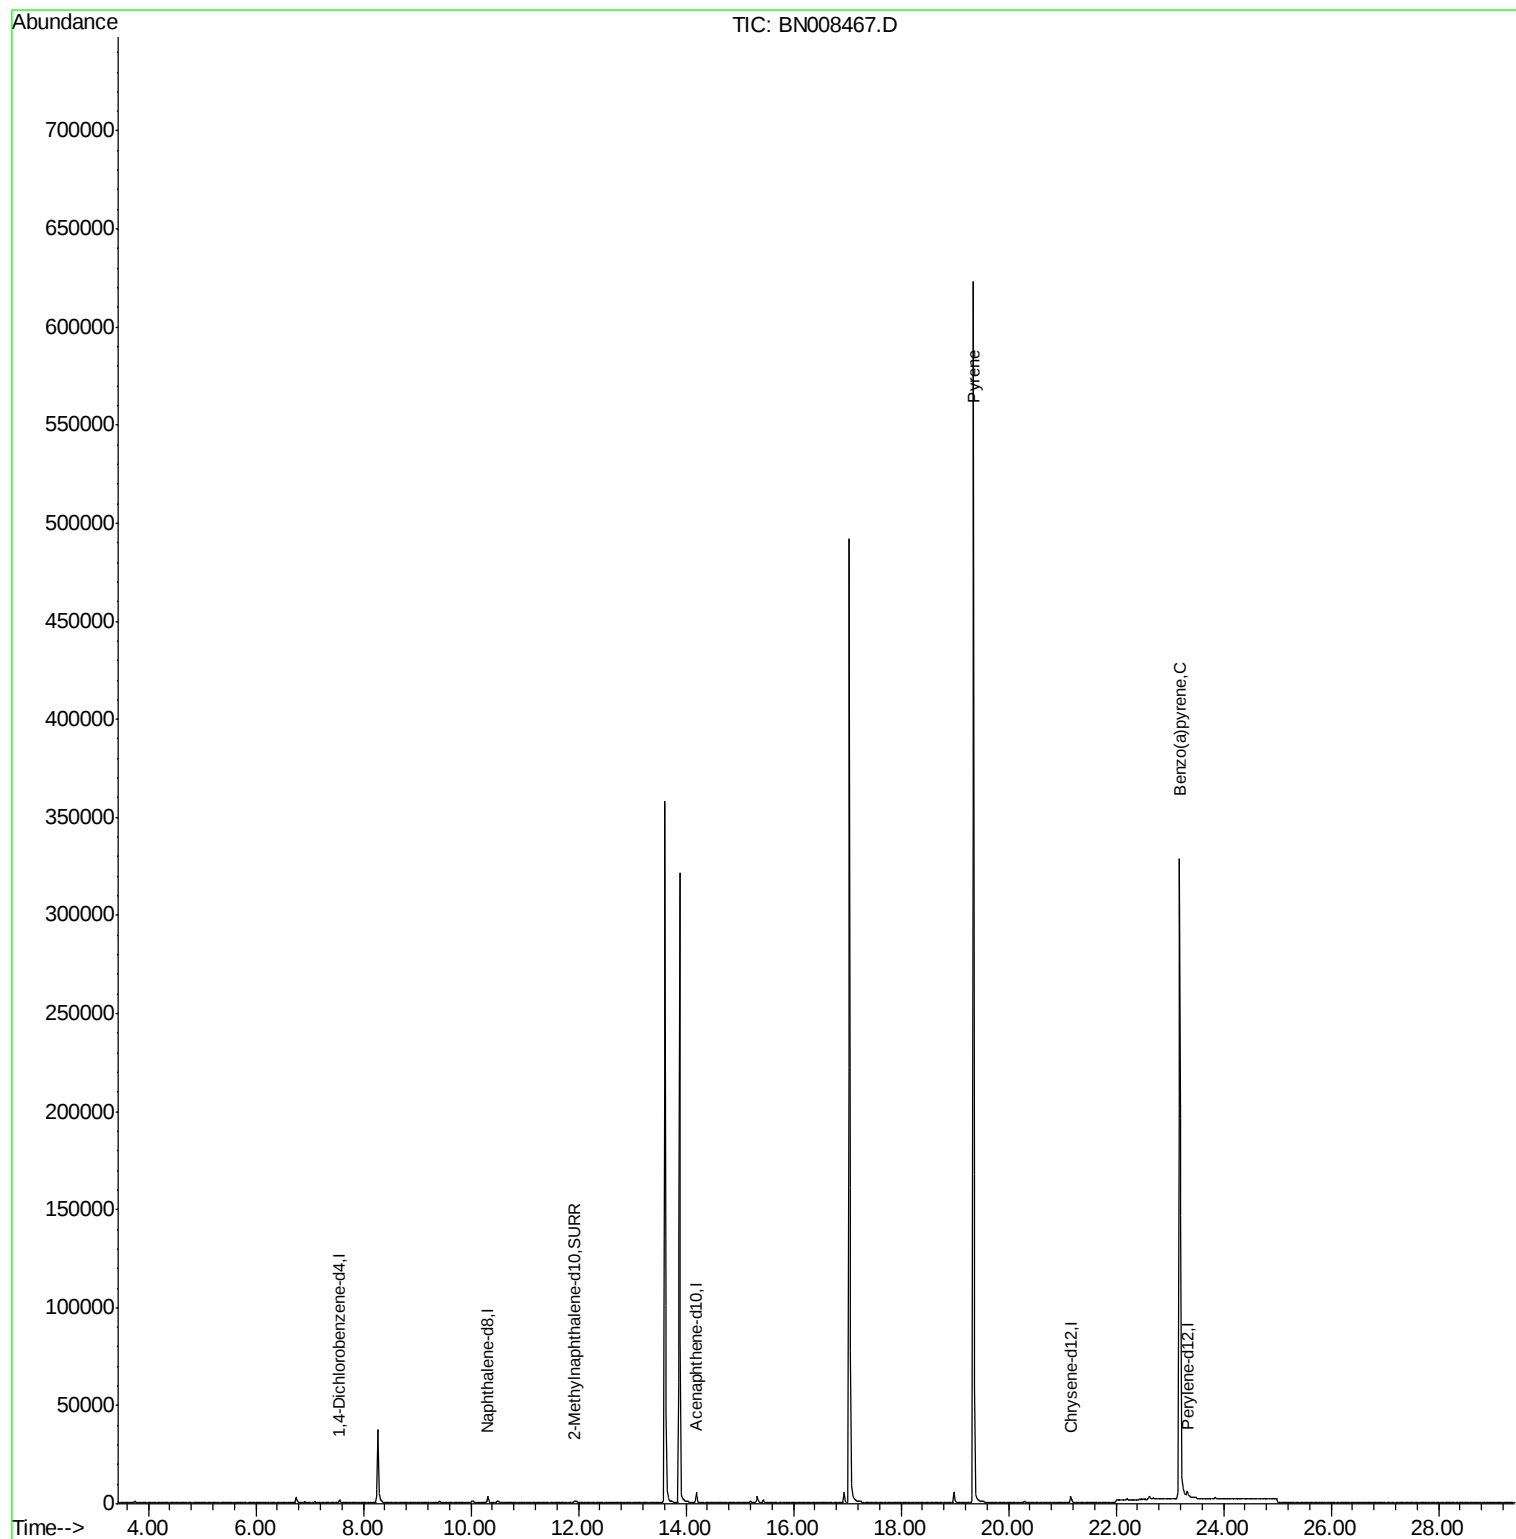

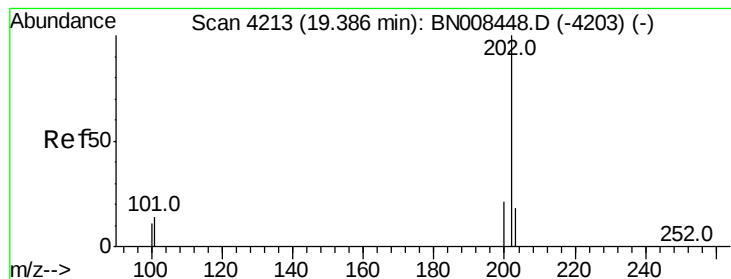

#17

Pvrene

Concen: 0.048 ng/ul

RT: 19.35 min Scan# 4205

Delta R.T. -0.04 min

Lab File: BN008467.D

Acq: 06 Nov 2019 15:23


Instrument :

BNA_N

ClientSampleId :

Tot Ion:202 Resp: 1079




Ion	Ratio	Lower	Upper
202	100		
101	189.0	11.6	17.4#
100	1314.4	9.4	14.0#

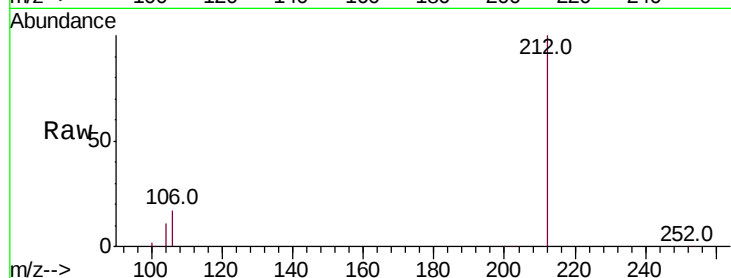

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

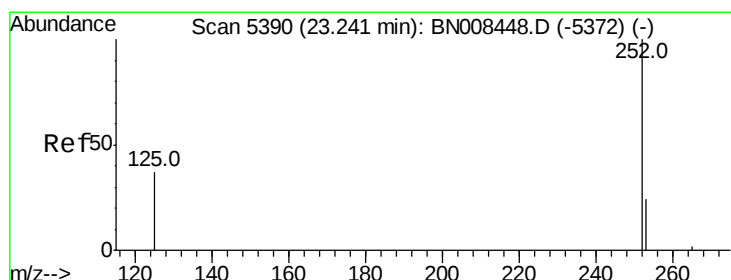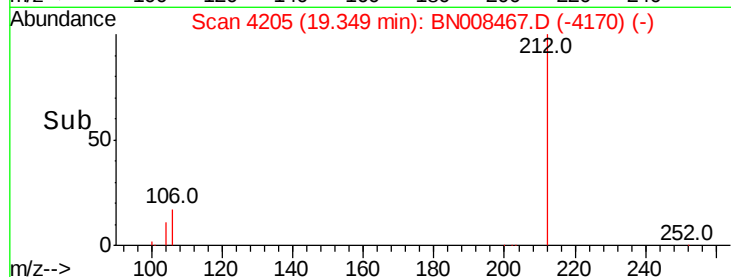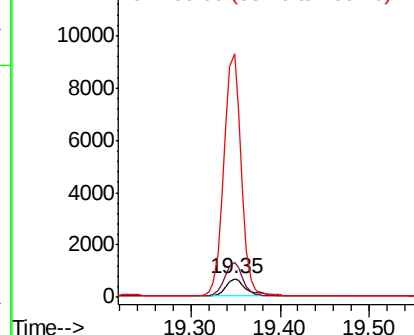

#23

Benzo(a)pyrene

Concen: 0.107 ng/ul

RT: 23.19 min Scan# 5371


Delta R.T. -0.06 min

Lab File: BN008467.D

Acq: 06 Nov 2019 15:23

Tgt Ion:252 Resp: 1627

Ion	Ratio	Lower	Upper
252	100		
253	51.7	27.2	40.8#
125	49.0	37.0	55.6

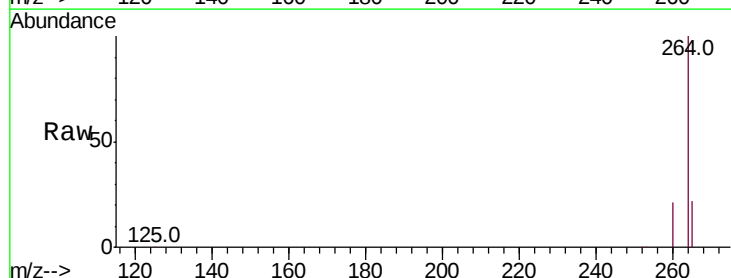

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

