

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
 Data File : BN008468.D
 Acq On : 06 Nov 2019 15:59
 Operator : JU
 Sample : K5656-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Nov 07 12:25:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 12:16:36 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	1294	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	5667	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.20	164	3373	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.95
16) Chrysene-d12	21.16	240	5277	0.40	ng/ul	0.00
20) Perylene-d12	23.32	264	4752	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.93	152	2341	0.26	ng/ul	0.02
14) Fluoranthene-d10	18.99	212	8047	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.35	202	1258	0.049	ng/ul#	1
23) Benzo(a)pyrene	23.18	252	1869	0.105	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
Data File : BN008468.D
Acq On : 06 Nov 2019 15:59
Operator : JU
Sample : K5656-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Nov 07 12:25:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 12:16:36 2019
Response via : Initial Calibration

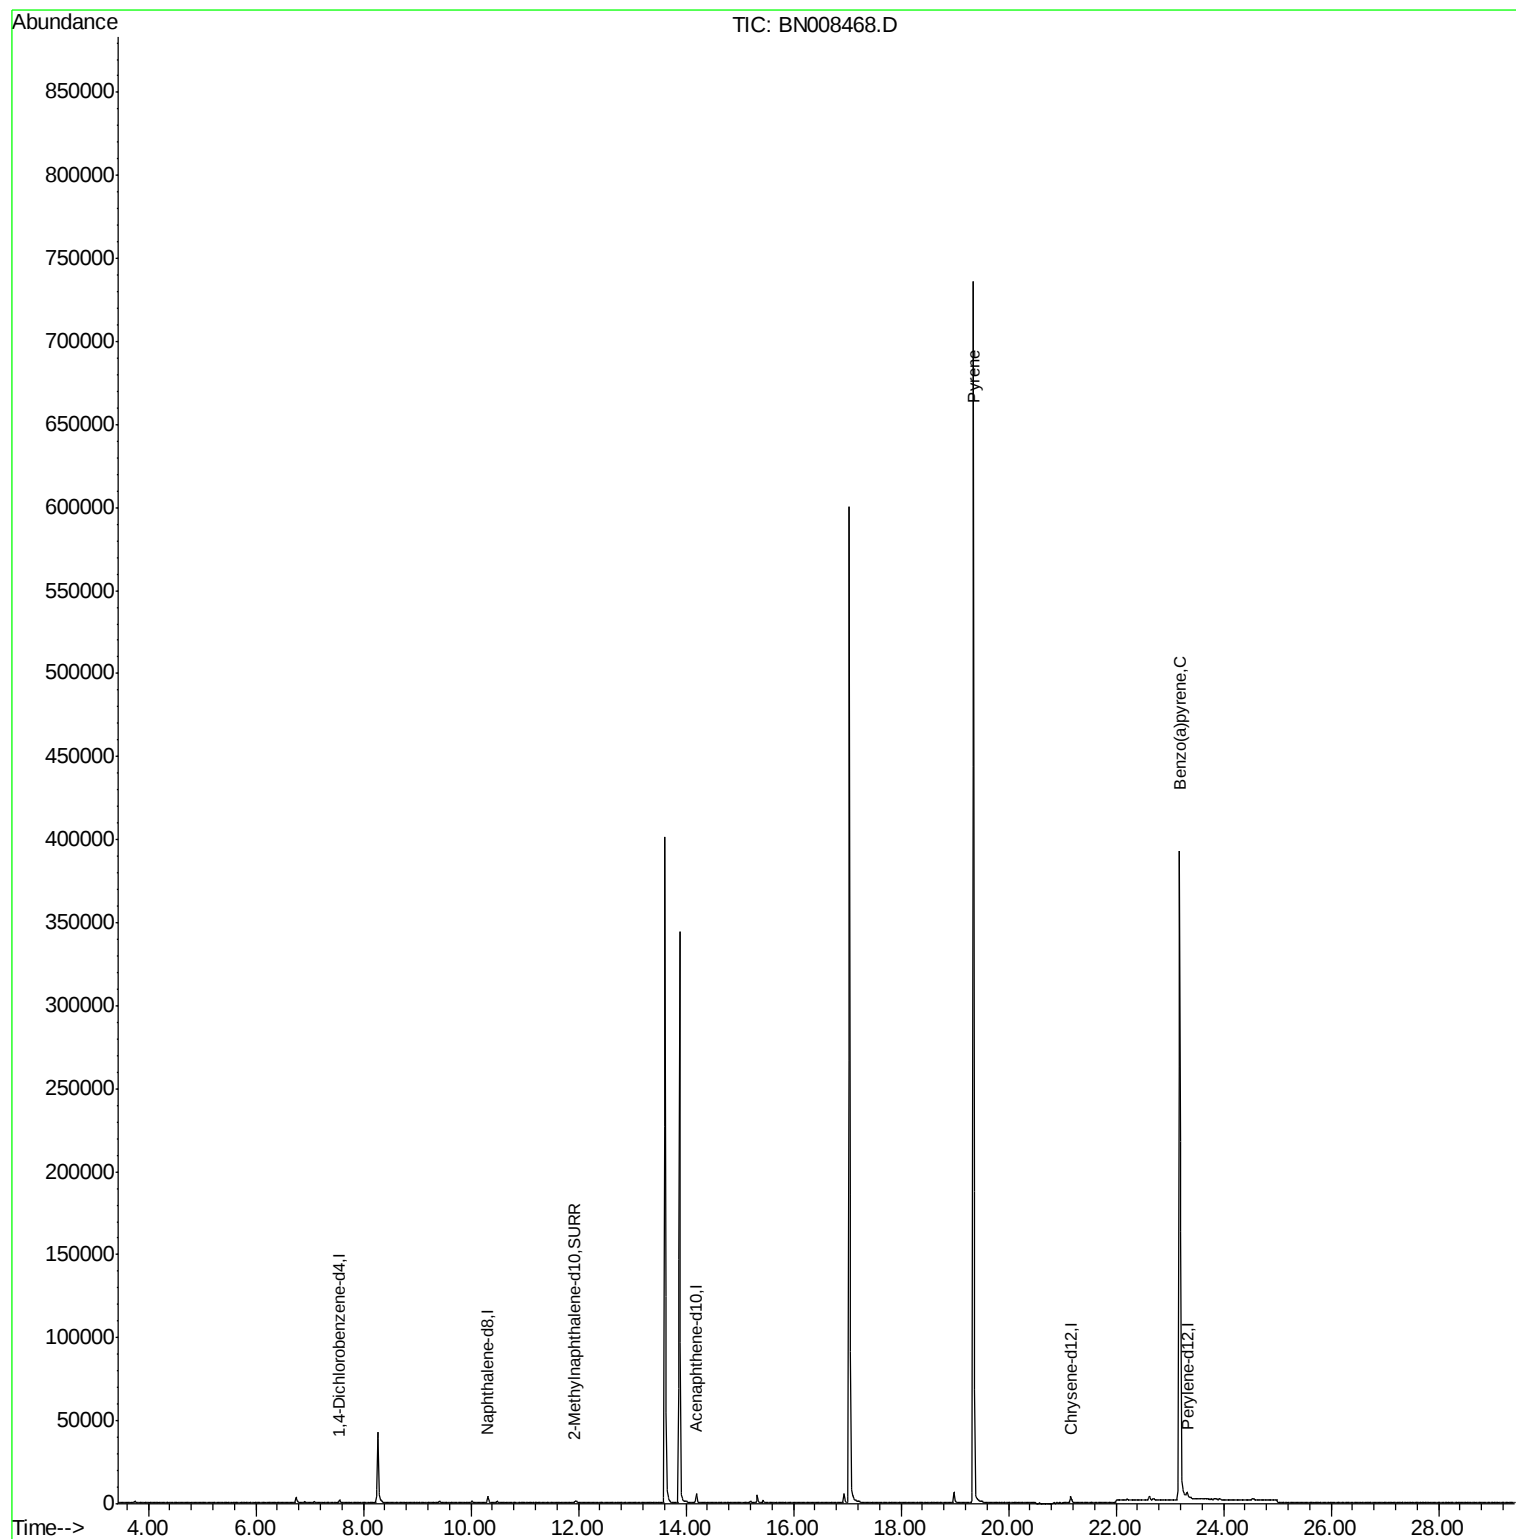


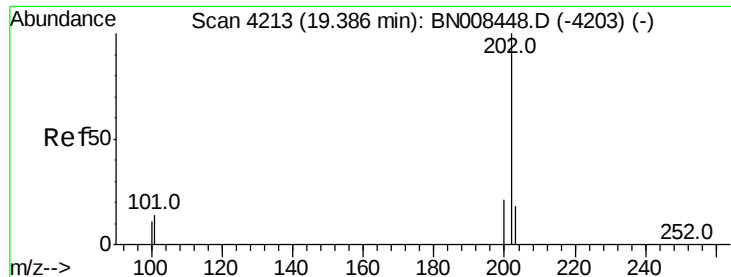




#17
Pvrene
Concen: 0.049 ng/ul
RT: 19.35 min Scan# 4205
Delta R.T. -0.04 min
Lab File: BN008468.D
Acq: 06 Nov 2019 15:59

Instrument :
BNA_N
ClientSampleId :

Tot Ion:202 Resp: 1258
Ion Ratio Lower Upper
202 100
101 183.6 11.6 17.4#
100 1245.1 9.4 14.0#

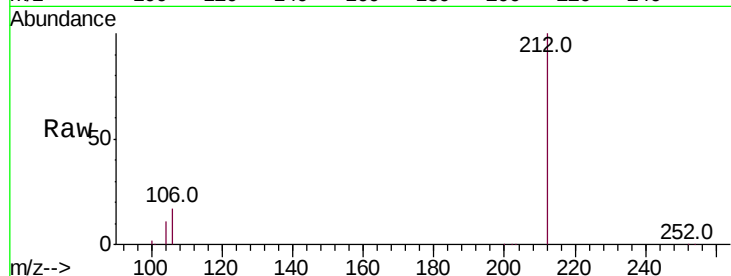

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

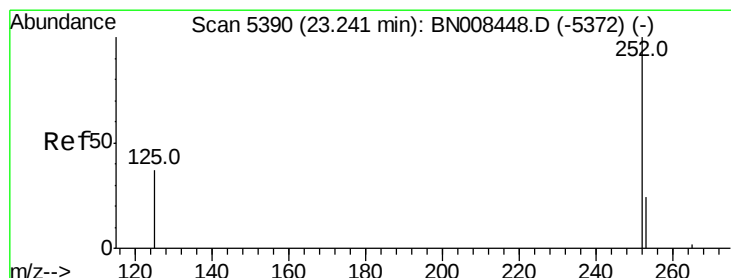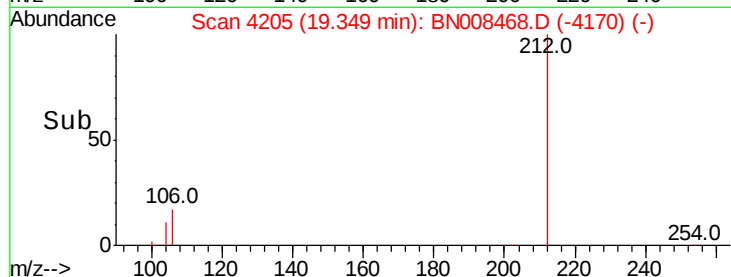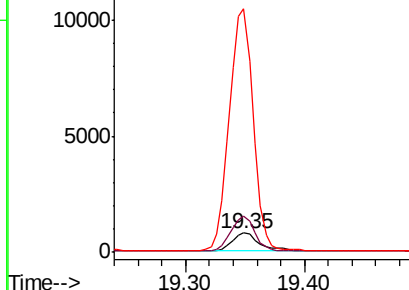

#23
Benzo(a)pyrene
Concen: 0.105 ng/ul
RT: 23.18 min Scan# 5370
Delta R.T. -0.06 min
Lab File: BN008468.D
Acq: 06 Nov 2019 15:59

Tgt Ion:252 Resp: 1869
Ion Ratio Lower Upper
252 100
253 48.0 27.2 40.8#
125 44.6 37.0 55.6

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

