

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
 Data File : BN008469.D
 Acq On : 06 Nov 2019 16:35
 Operator : JU
 Sample : K5656-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Nov 07 12:25:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 12:16:36 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	1294	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	5663	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	3364	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.95
16) Chrysene-d12	21.16	240	5249	0.40	ng/ul	0.00
20) Perylene-d12	23.33	264	4749	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.93	152	2272	0.25	ng/ul	0.02
14) Fluoranthene-d10	18.99	212	7531	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.35	202	1134	0.044	ng/ul#	1
23) Benzo(a)pyrene	23.19	252	1818	0.102	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
Data File : BN008469.D
Acq On : 06 Nov 2019 16:35
Operator : JU
Sample : K5656-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Nov 07 12:25:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 12:16:36 2019
Response via : Initial Calibration

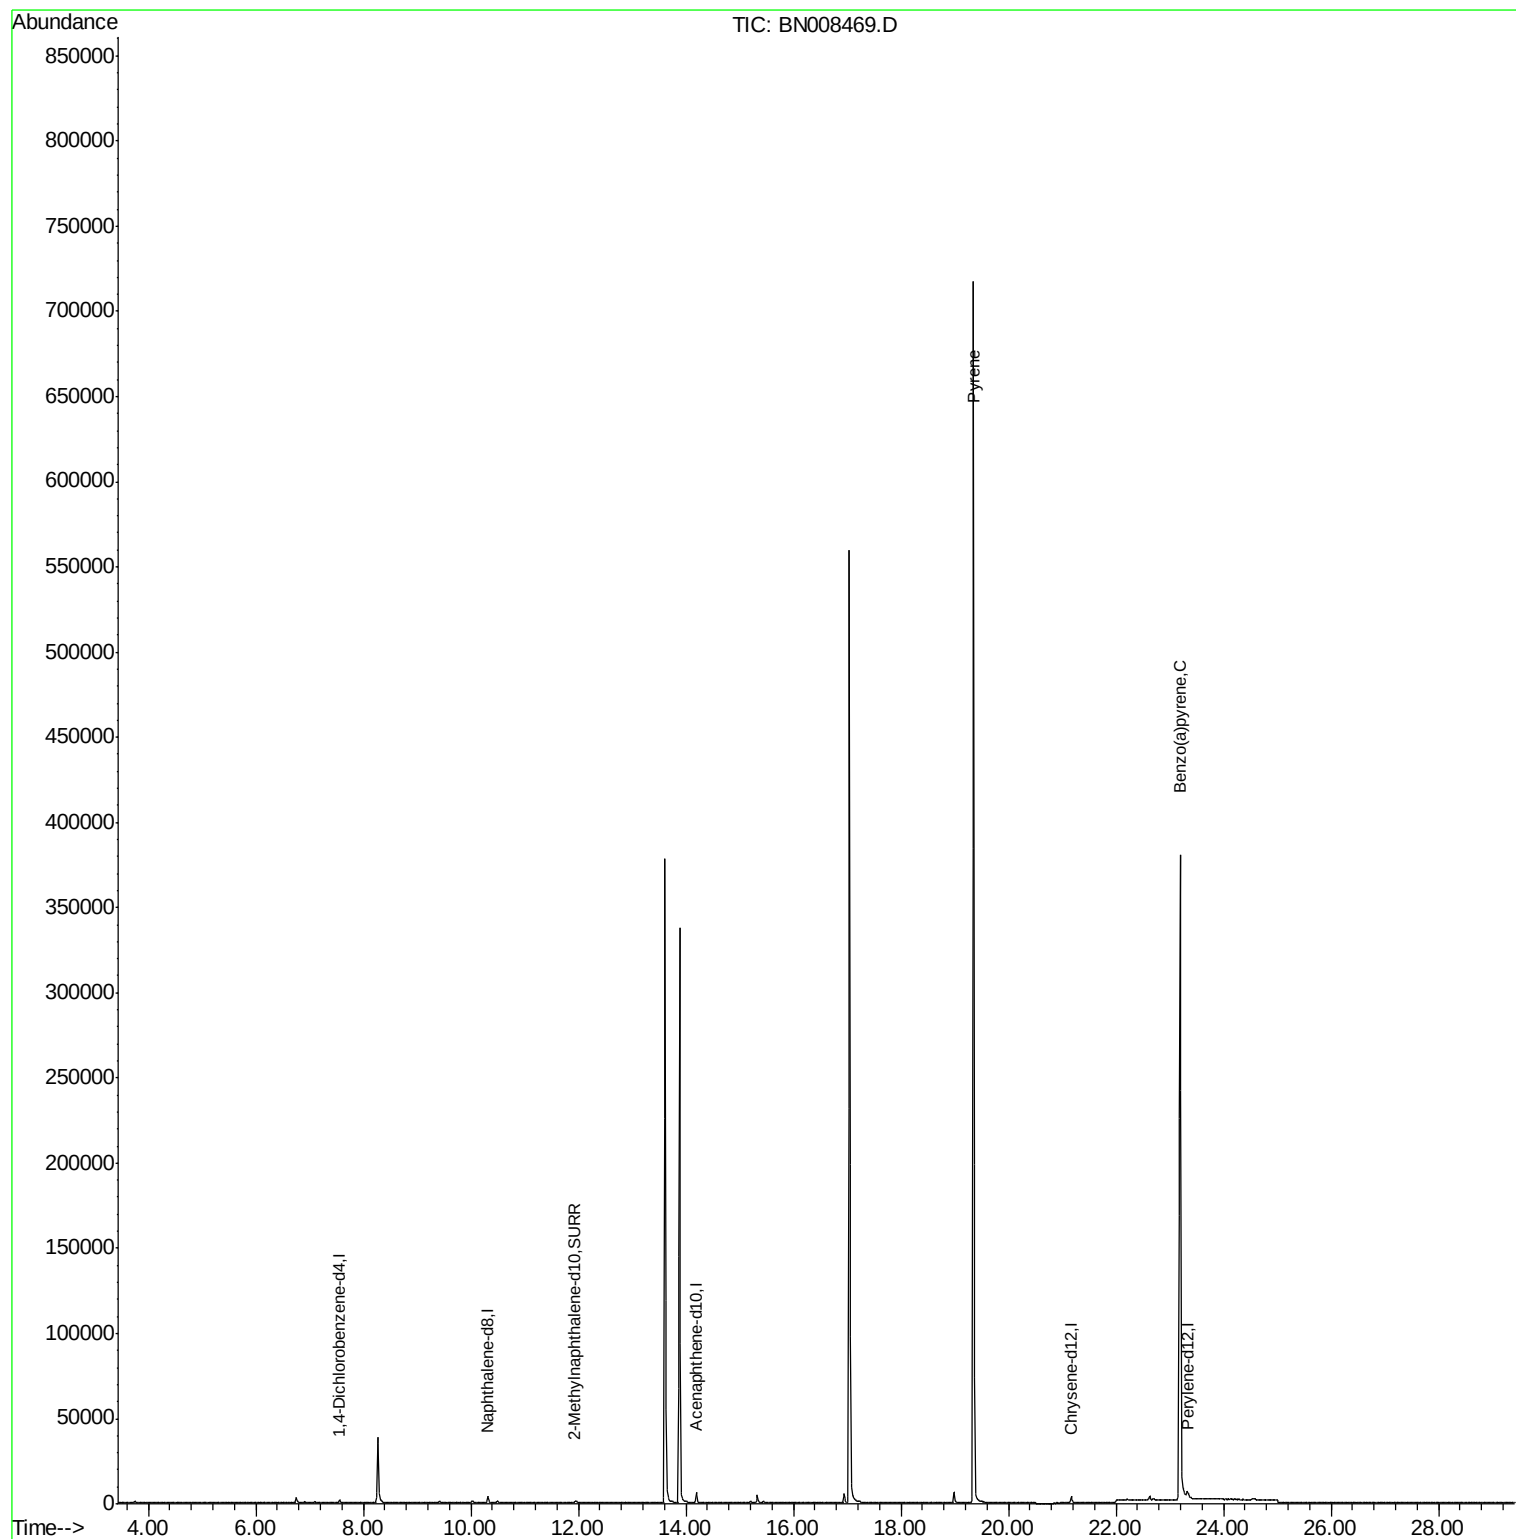

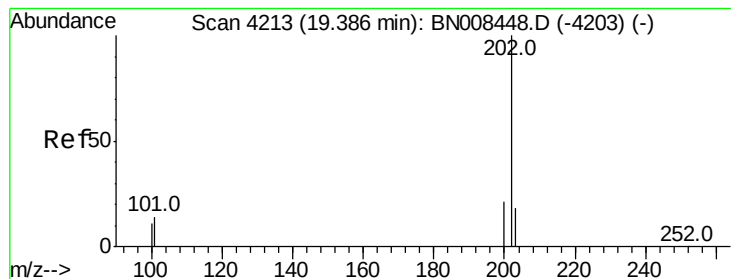

#17

Pvrene

Concen: 0.044 ng/ul

RT: 19.35 min Scan# 4205

Delta R.T. -0.04 min

Lab File: BN008469.D

Acq: 06 Nov 2019 16:35

Instrument :

BNA_N

ClientSampleId :


Tot Ion:202 Resp: 1134

Ion Ratio Lower Upper

202 100

101 179.7 11.6 17.4#




100 1237.8 9.4 14.0#

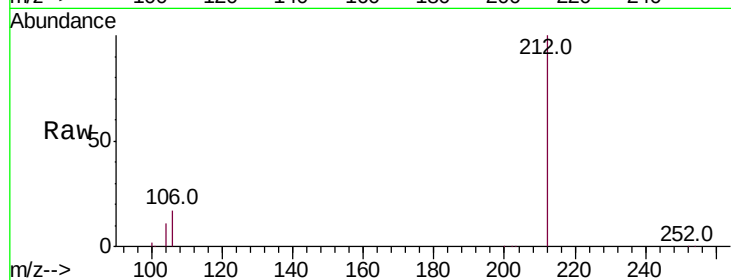

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

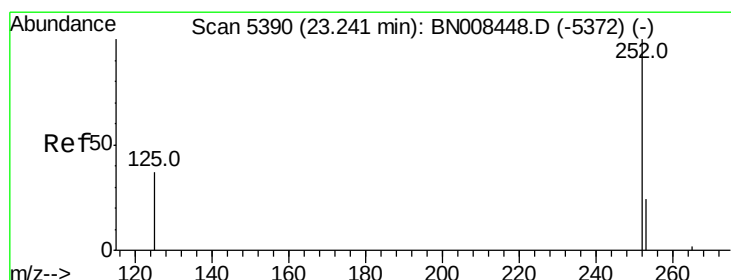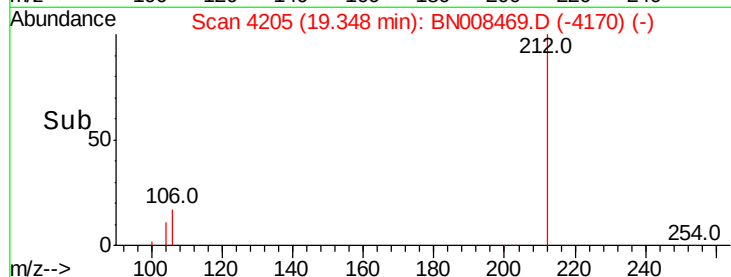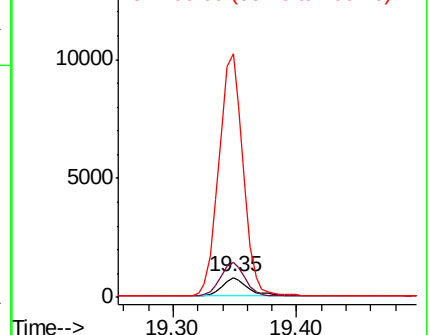

#23

Benzo(a)pyrene

Concen: 0.102 ng/ul

RT: 23.19 min Scan# 5372

Delta R.T. -0.05 min

Lab File: BN008469.D

Acq: 06 Nov 2019 16:35


Tgt Ion:252 Resp: 1818

Ion Ratio Lower Upper

252 100

253 47.1 27.2 40.8#

125 44.0 37.0 55.6

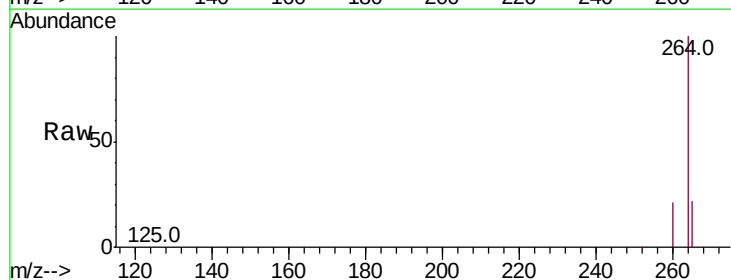

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

