

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
 Data File : BN008473.D
 Acq On : 06 Nov 2019 18:58
 Operator : JU
 Sample : K5656-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Nov 07 12:25:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 12:16:36 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	1248	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	5435	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	3256	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.95
16) Chrysene-d12	21.16	240	5457	0.40	ng/ul	0.00
20) Perylene-d12	23.32	264	5302	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.93	152	2178	0.25	ng/ul	0.02
14) Fluoranthene-d10	18.98	212	7185	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.19	166	958	0.071	ng/ul#	17
17) Pyrene	19.35	202	1011	0.038	ng/ul#	1
23) Benzo(a)pyrene	23.18	252	1758	0.088	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
Data File : BN008473.D
Acq On : 06 Nov 2019 18:58
Operator : JU
Sample : K5656-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Nov 07 12:25:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 12:16:36 2019
Response via : Initial Calibration




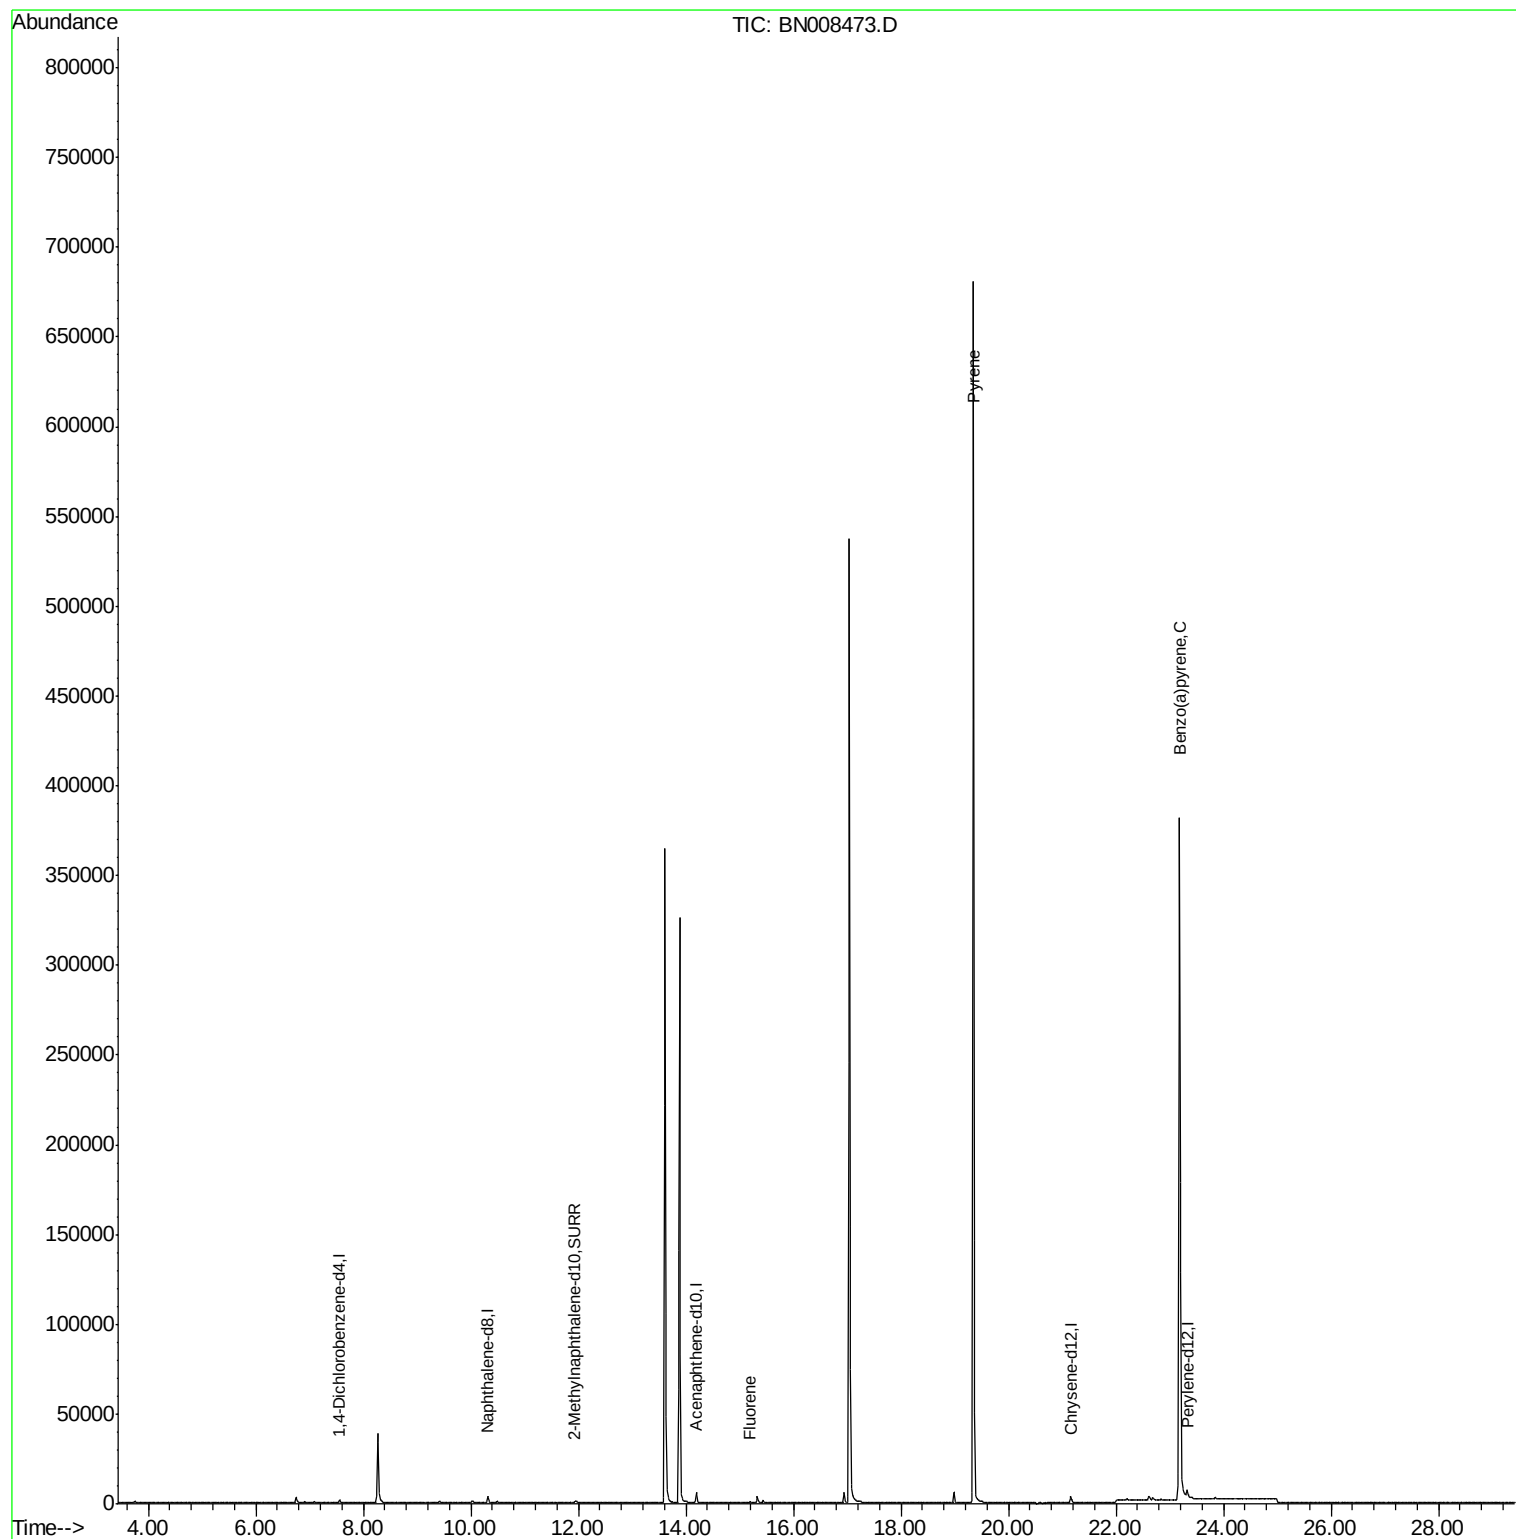


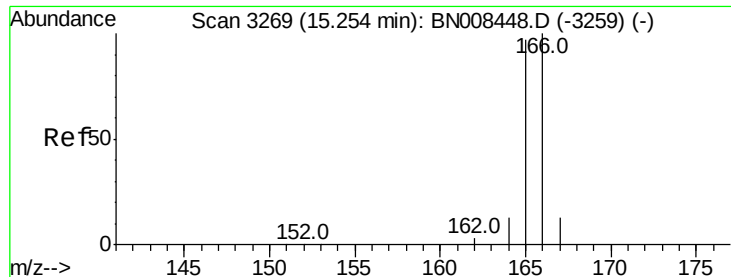

#9
Fluorene
Concen: 0.071 ng/ul
RT: 15.19 min Scan# 3256
Delta R.T. -0.06 min
Lab File: BN008473.D
Acq: 06 Nov 2019 18:58




Instrument :
BNA_N
ClientSampleId :


Tot Ion:166 Resp: 958
Ion Ratio Lower Upper
166 100
165 11.1 78.2 117.2#
167 37.6 12.1 18.1#

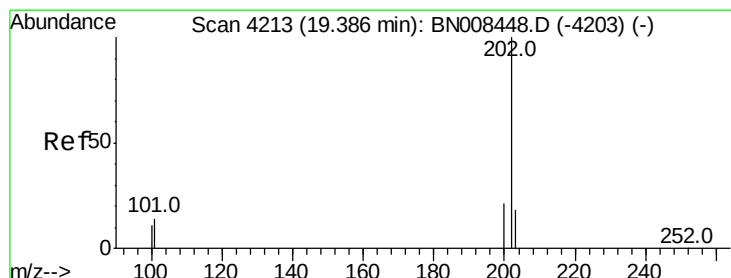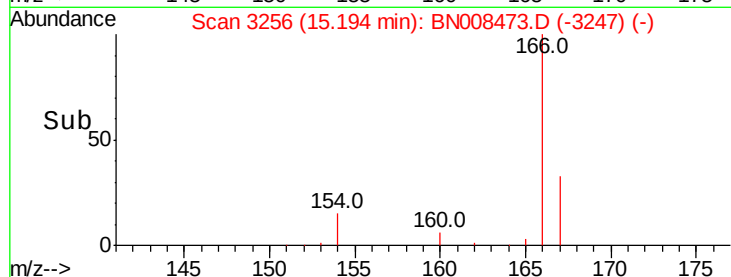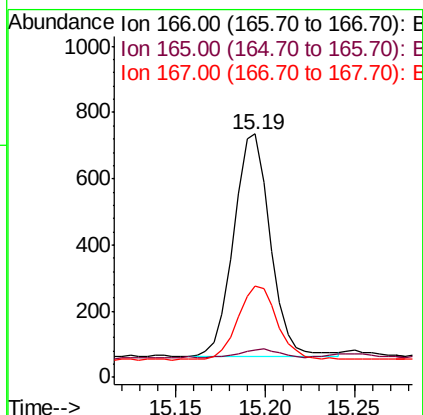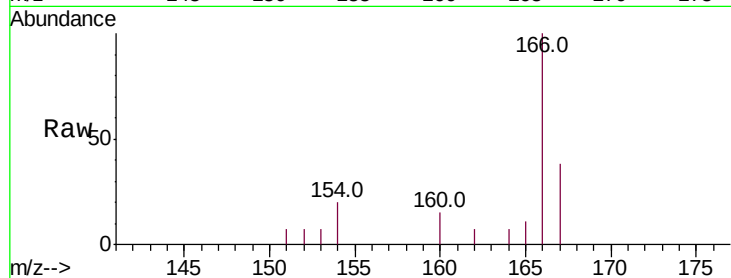

#17
Pyrene
Concen: 0.038 ng/ul
RT: 19.35 min Scan# 4205
Delta R.T. -0.04 min
Lab File: BN008473.D
Acq: 06 Nov 2019 18:58

Tgt Ion:202 Resp: 1011
Ion Ratio Lower Upper
202 100
101 185.2 11.6 17.4#
100 1240.1 9.4 14.0#

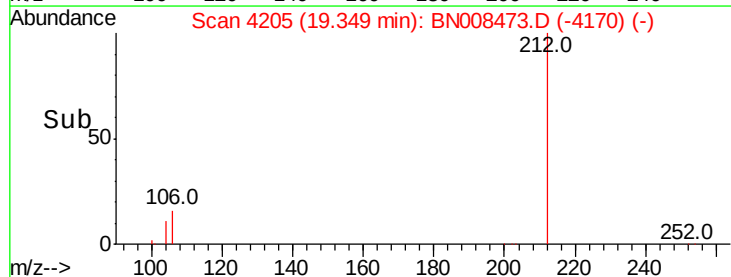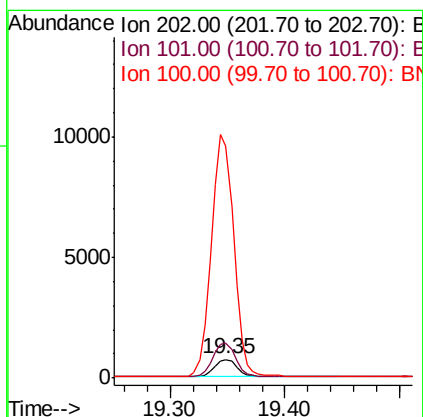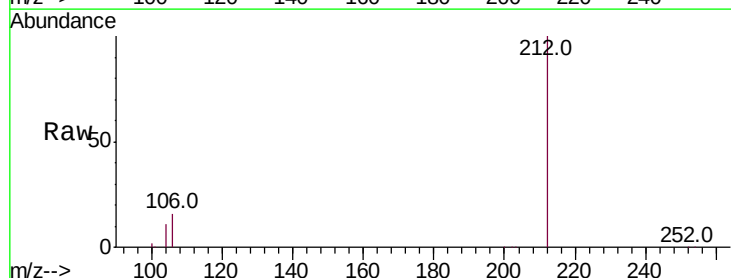

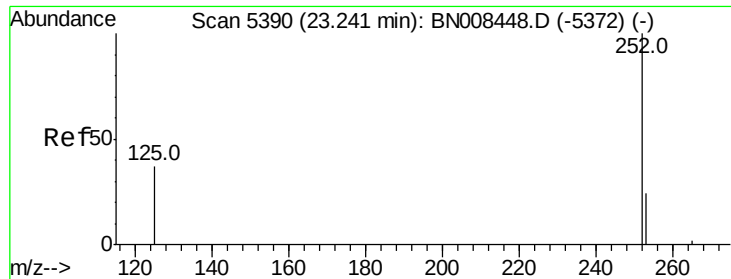

#23

Benzo(a)pyrene

Concen: 0.088 ng/ul

RT: 23.18 min Scan# 5370

Delta R.T. -0.06 min

Lab File: BN008473.D

Acq: 06 Nov 2019 18:58

Instrument :

BNA_N

ClientSampleId :


Tot Ion: 252 Resp: 1758

Ion Ratio Lower Upper

252 100

253 48.7 27.2 40.8#

125 45.7 37.0 55.6

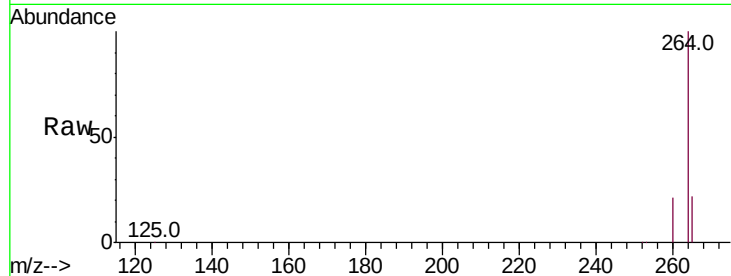

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

