

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
 Data File : BN008475.D
 Acq On : 06 Nov 2019 20:09
 Operator : JU
 Sample : PB124532BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Nov 07 12:25:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 12:16:36 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	1423	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	6191	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	3656	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.95
16) Chrysene-d12	21.17	240	5278	0.40	ng/ul	0.00
20) Perylene-d12	23.32	264	5725	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.94	152	2934	0.30	ng/ul	0.02
14) Fluoranthene-d10	18.99	212	7781	0.00	ng/ul	0.00
Target Compounds						
					Ovalue	
9) Fluorene	15.19	166	1187	0.079	ng/ul#	16
17) Pyrene	19.35	202	1114	0.043	ng/ul#	1
23) Benzo(a)pyrene	23.18	252	1827	0.085	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
Data File : BN008475.D
Acq On : 06 Nov 2019 20:09
Operator : JU
Sample : PB124532BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Nov 07 12:25:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 12:16:36 2019
Response via : Initial Calibration




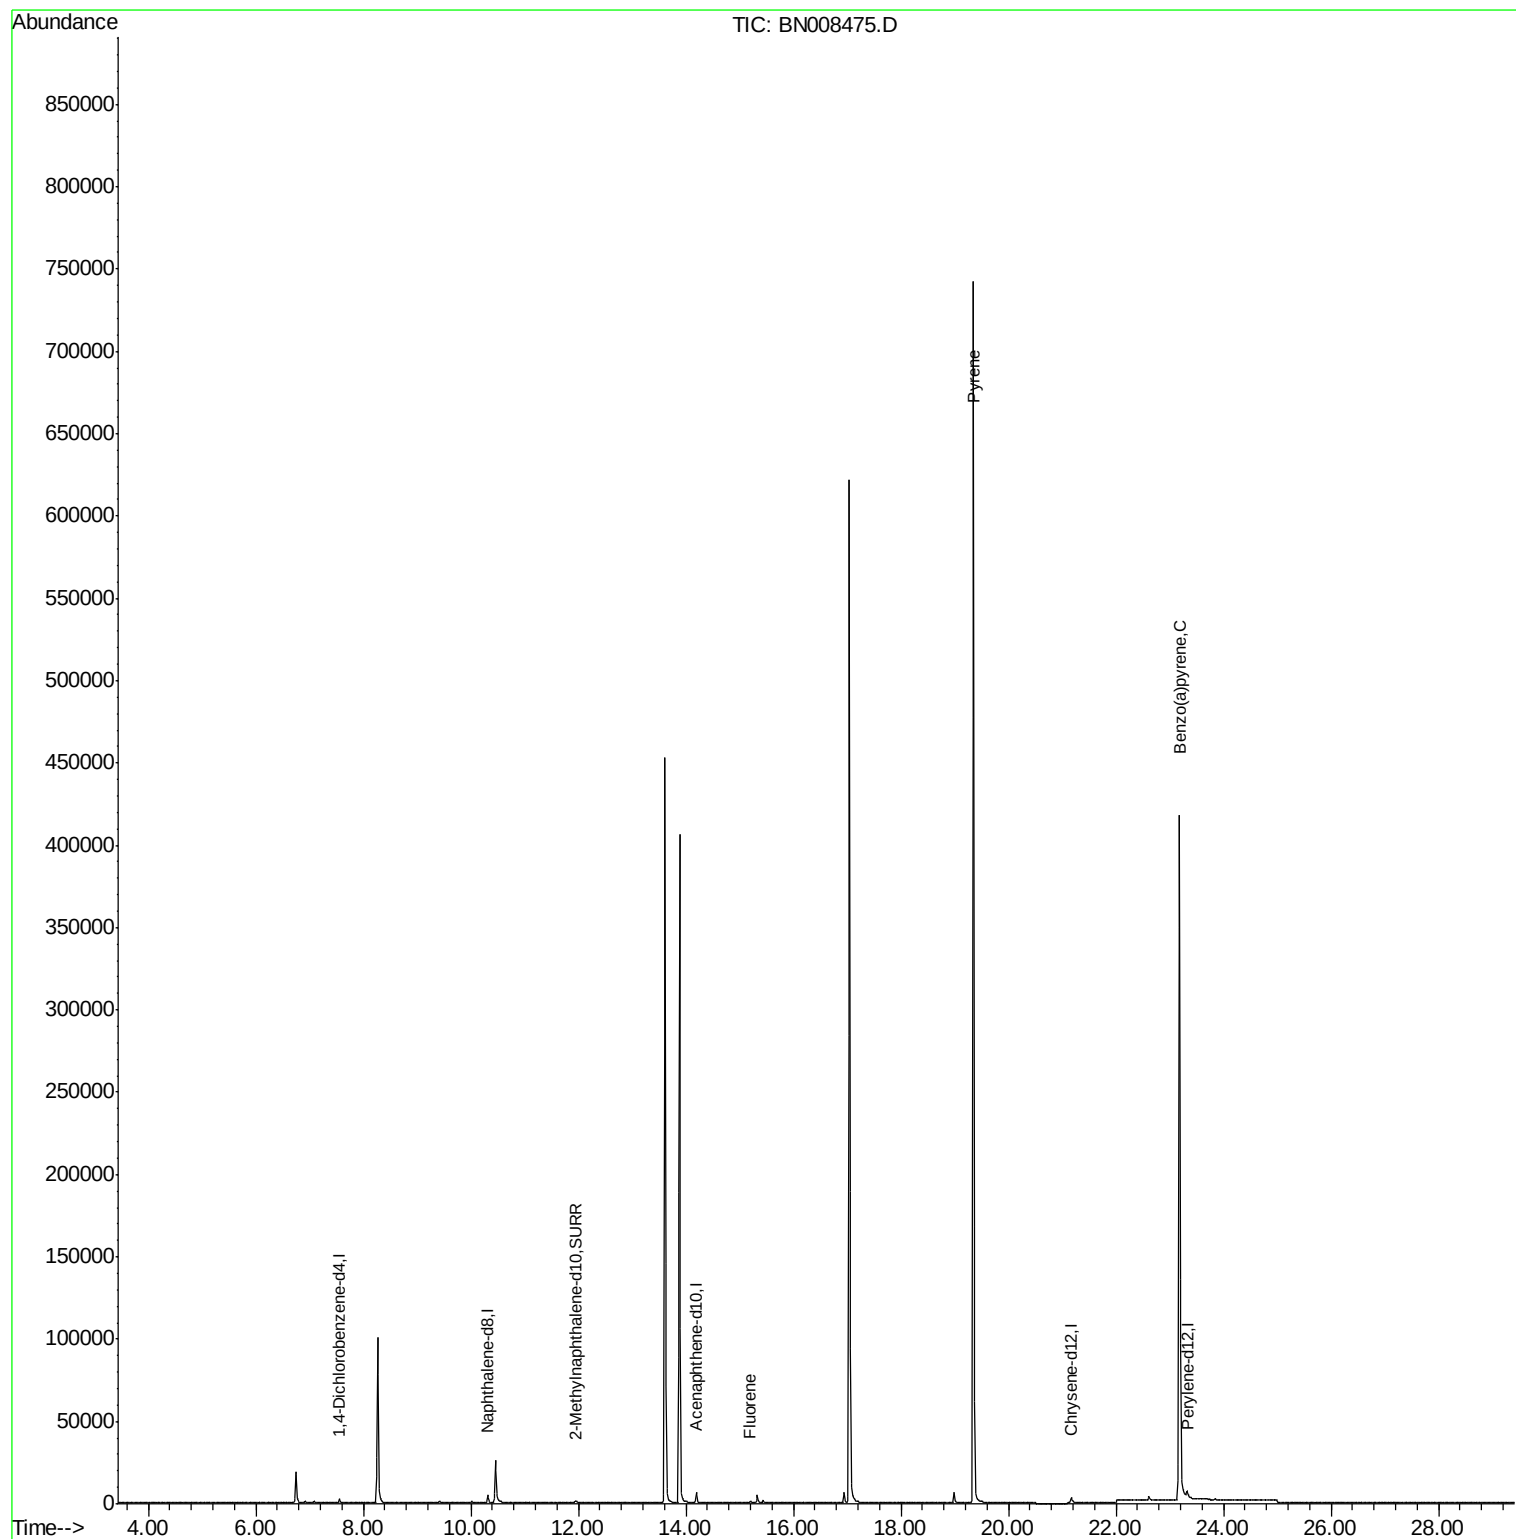


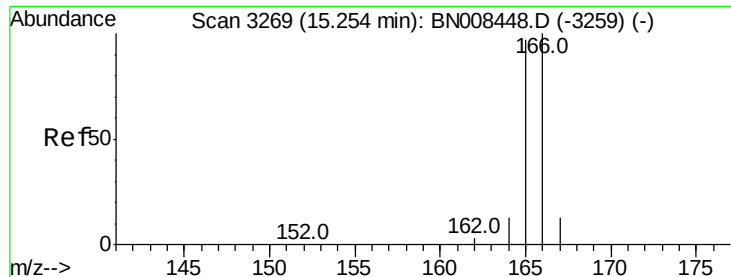

#9
Fluorene
Concen: 0.079 ng/ul
RT: 15.19 min Scan# 3256
Delta R.T. -0.06 min
Lab File: BN008475.D
Acq: 06 Nov 2019 20:09




Instrument :
BNA_N
ClientSampleId :


Tot Ion:166 Resp: 1187
Ion Ratio Lower Upper
166 100
165 10.0 78.2 117.2#
167 36.6 12.1 18.1#

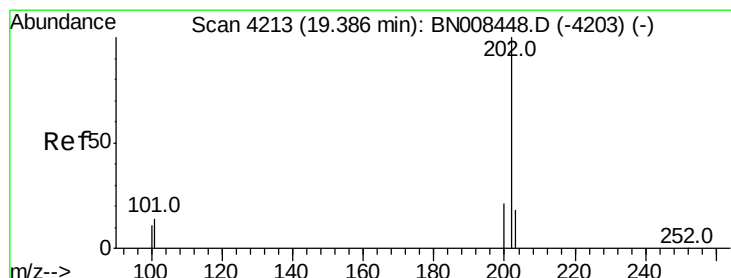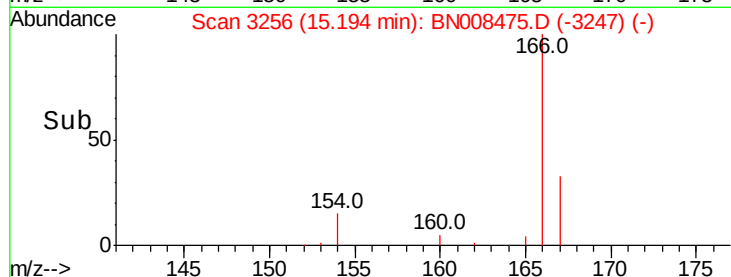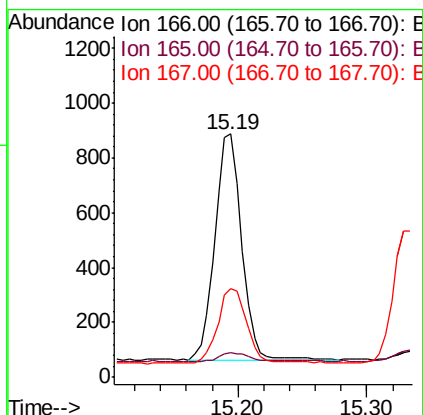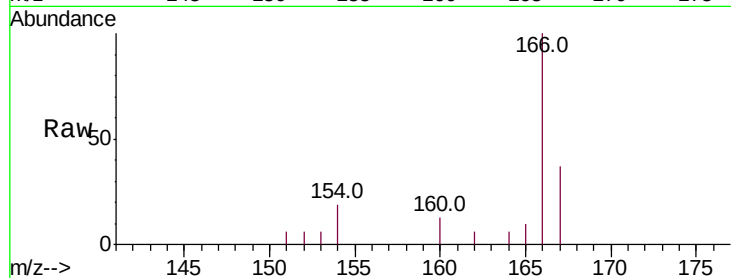

#17
Pyrene
Concen: 0.043 ng/ul
RT: 19.35 min Scan# 4205
Delta R.T. -0.04 min
Lab File: BN008475.D
Acq: 06 Nov 2019 20:09

Tgt Ion:202 Resp: 1114
Ion Ratio Lower Upper
202 100
101 184.8 11.6 17.4#
100 1244.7 9.4 14.0#

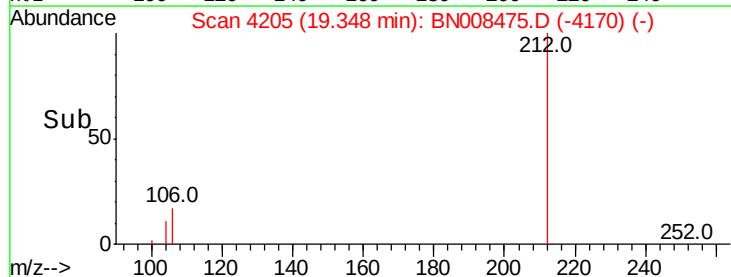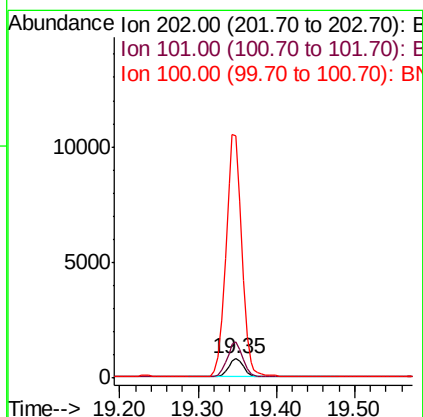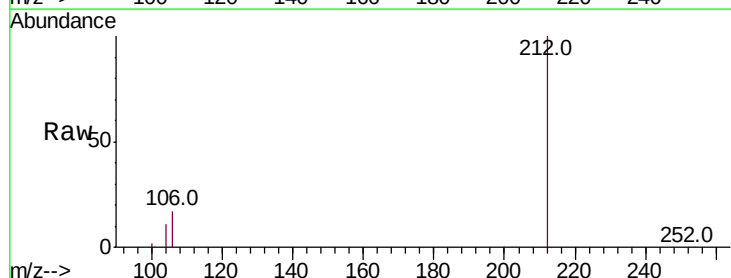

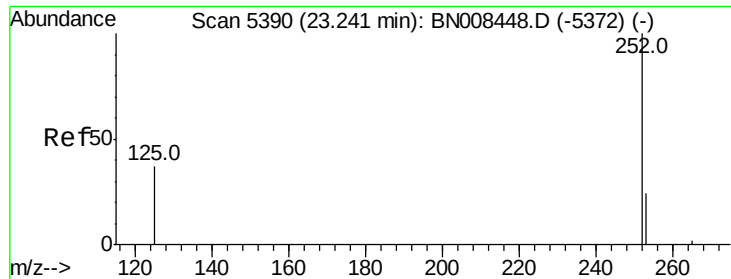

#23

Benzo(a)pyrene

Concen: 0.085 ng/ul

RT: 23.18 min Scan# 5369

Delta R.T. -0.06 min

Lab File: BN008475.D

Acq: 06 Nov 2019 20:09

Instrument :

BNA_N

ClientSampleId :


Tot Ion:252 Resp: 1827

Ion Ratio Lower Upper

252 100

253 46.9 27.2 40.8#

125 42.2 37.0 55.6

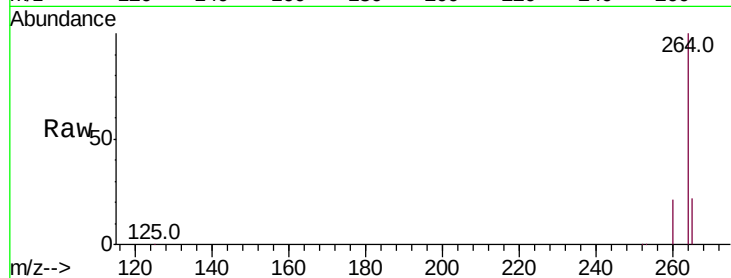

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

