

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
 Data File : BN008476.D
 Acq On : 06 Nov 2019 20:45
 Operator : JU
 Sample : PB124530BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Nov 07 12:25:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 12:16:36 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	1434	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	6153	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	3701	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.95
16) Chrysene-d12	21.16	240	5587	0.40	ng/ul	0.00
20) Perylene-d12	23.32	264	5269	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.93	152	2920	0.30	ng/ul	0.02
14) Fluoranthene-d10	18.99	212	8124	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.35	202	1236	0.045	ng/ul#	1
23) Benzo(a)pyrene	23.18	252	1951	0.099	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
Data File : BN008476.D
Acq On : 06 Nov 2019 20:45
Operator : JU
Sample : PB124530BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Nov 07 12:25:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 12:16:36 2019
Response via : Initial Calibration

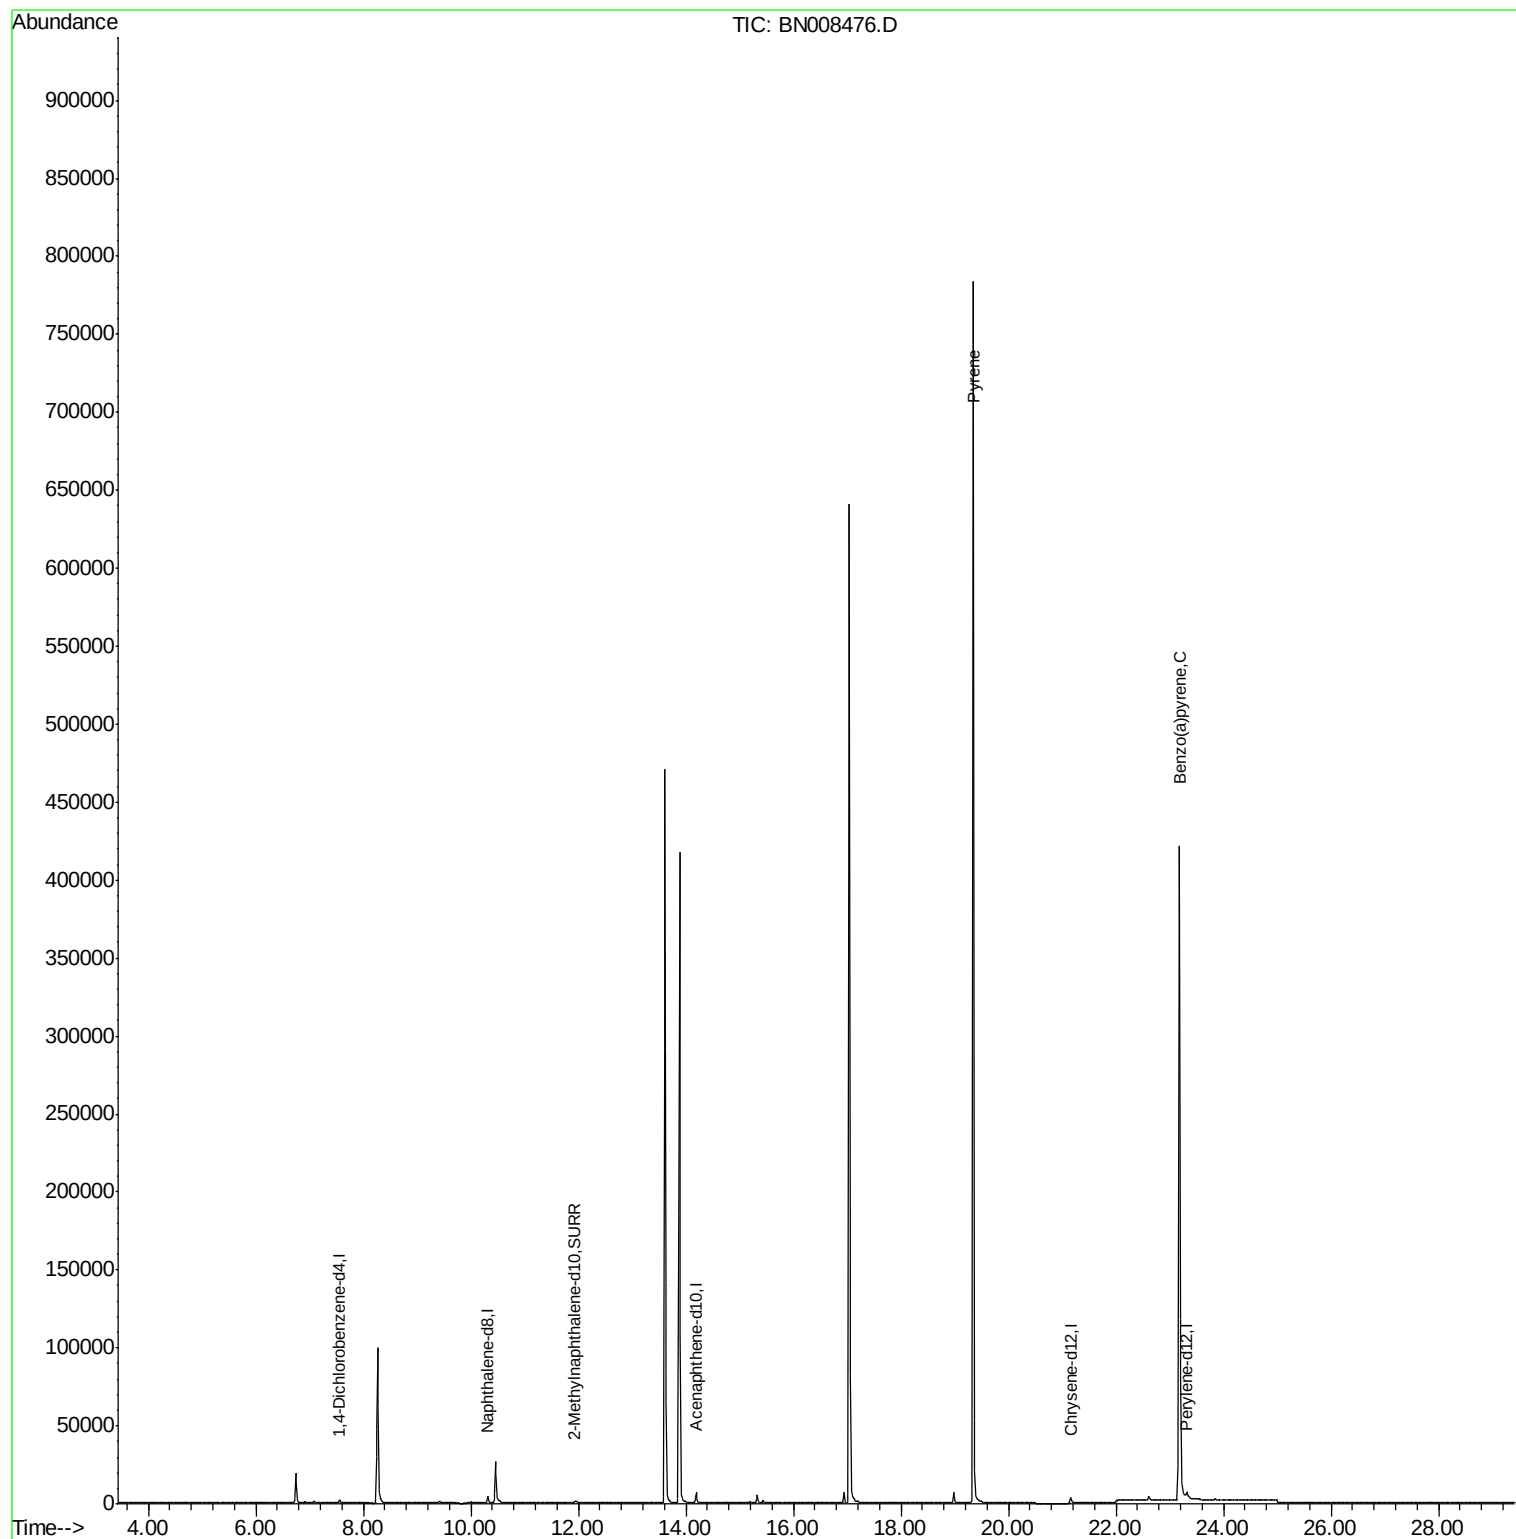

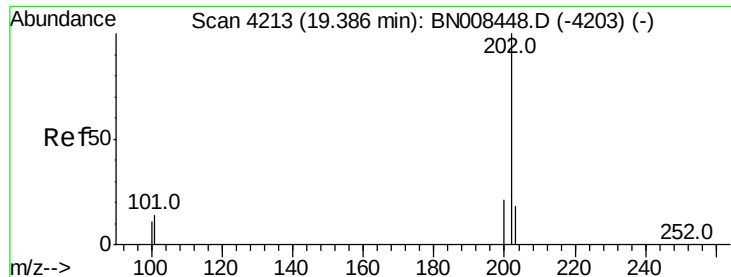

#17

Pvrene

Concen: 0.045 ng/ul

RT: 19.35 min Scan# 4205

Delta R.T. -0.04 min

Lab File: BN008476.D

Acq: 06 Nov 2019 20:45

Instrument :

BNA_N

ClientSampleId :


Tot Ion:202 Resp: 1236

Ion Ratio Lower Upper

202 100

101 182.5 11.6 17.4#




100 1232.8 9.4 14.0#

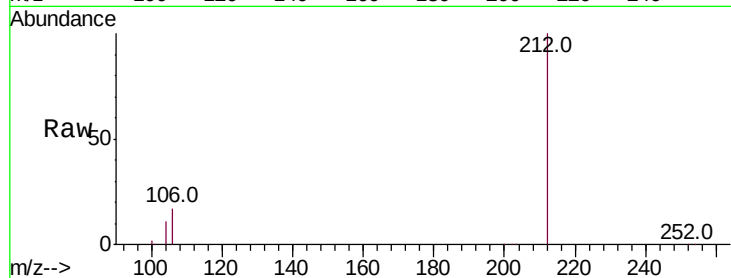

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

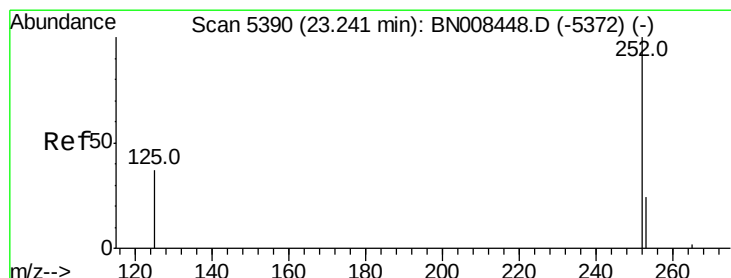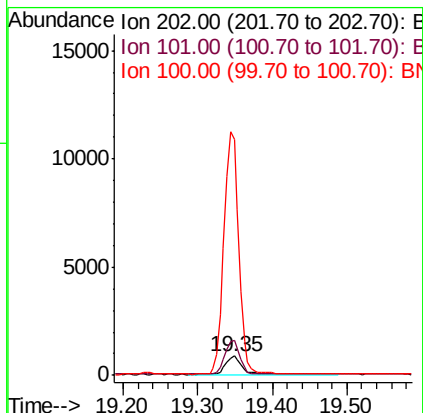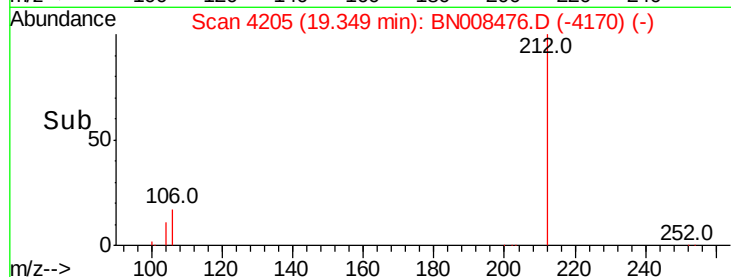

#23

Benzo(a)pyrene

Concen: 0.099 ng/ul

RT: 23.18 min Scan# 5369

Delta R.T. -0.06 min

Lab File: BN008476.D

Acq: 06 Nov 2019 20:45


Tgt Ion:252 Resp: 1951

Ion Ratio Lower Upper

252 100

253 45.8 27.2 40.8#

125 42.7 37.0 55.6

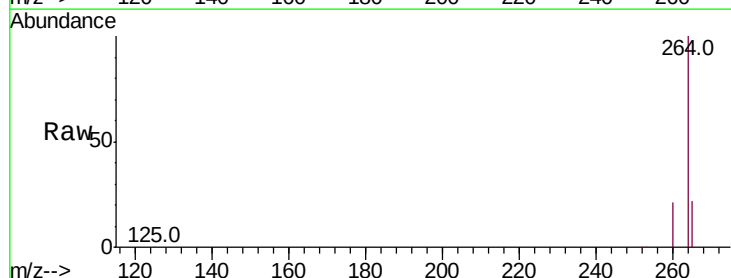

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

