


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
Data File : BN008473.D
Acq On : 06 Nov 2019 18:58
Operator : JU
Sample : K5656-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5454

Manual Integrations
APPROVED

Sohil
11/8/2019 3:29:18 PM

Quant Time: Nov 07 12:40:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 12:16:36 2019
Response via : Initial Calibration

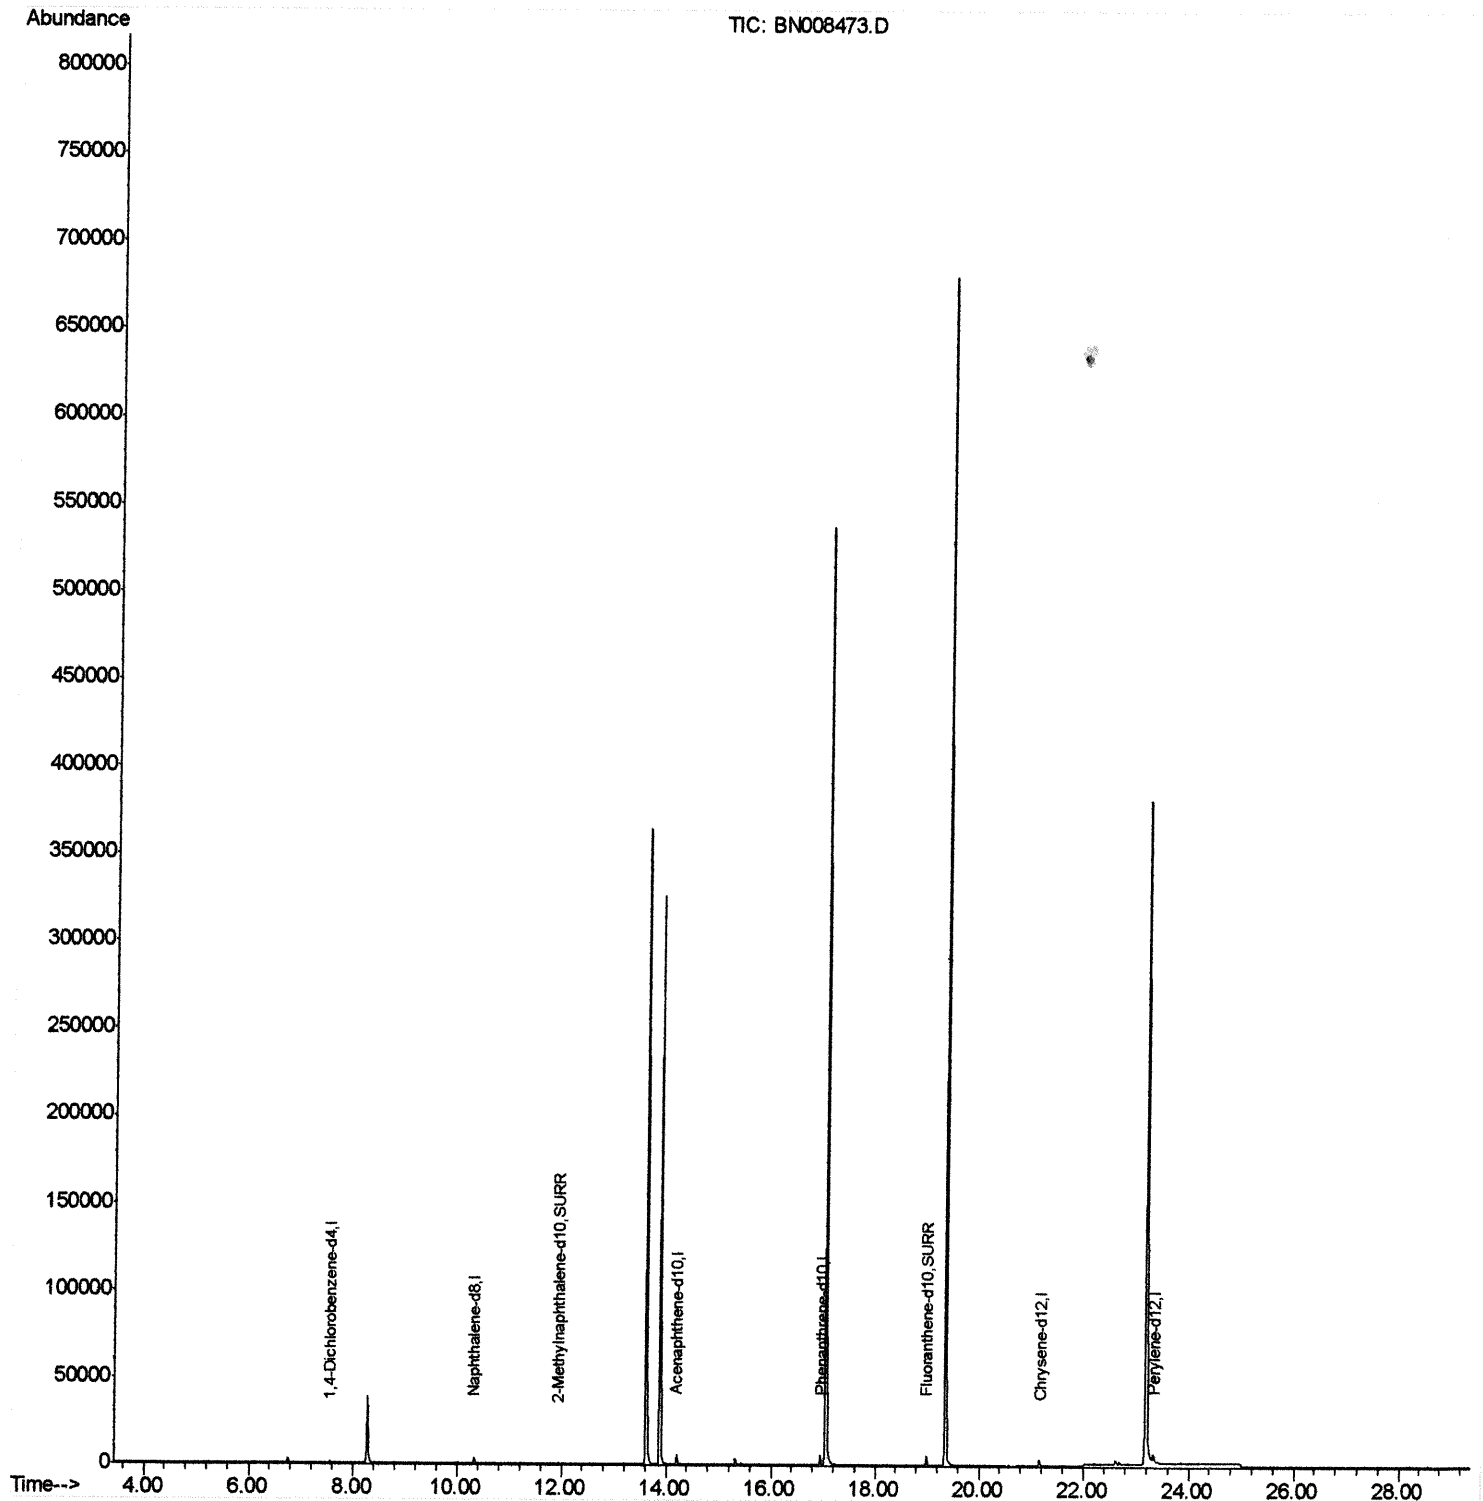

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
 Data File : BN008473.D
 Acq On : 06 Nov 2019 18:58
 Operator : JU
 Sample : K5656-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5454

Manual Integrations
 APPROVED

Sohil
 11/8/2019 3:29:18 PM

Quant Time: Nov 07 12:25:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 12:16:36 2019
 Response via : Initial Calibration

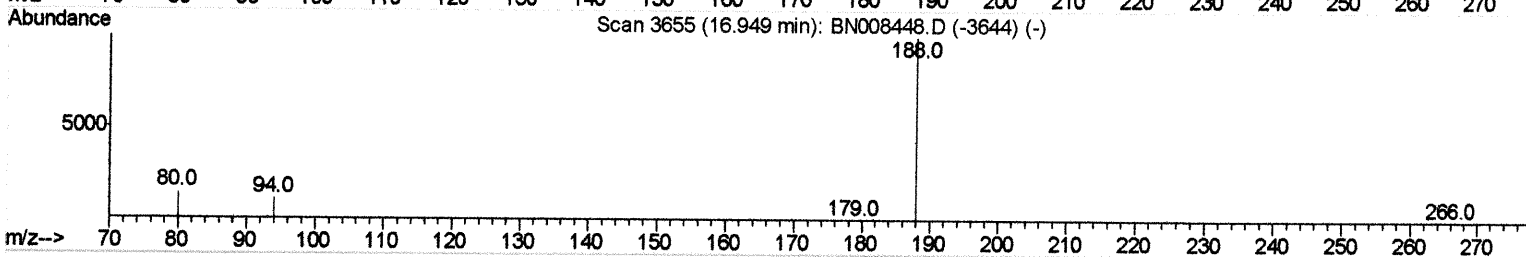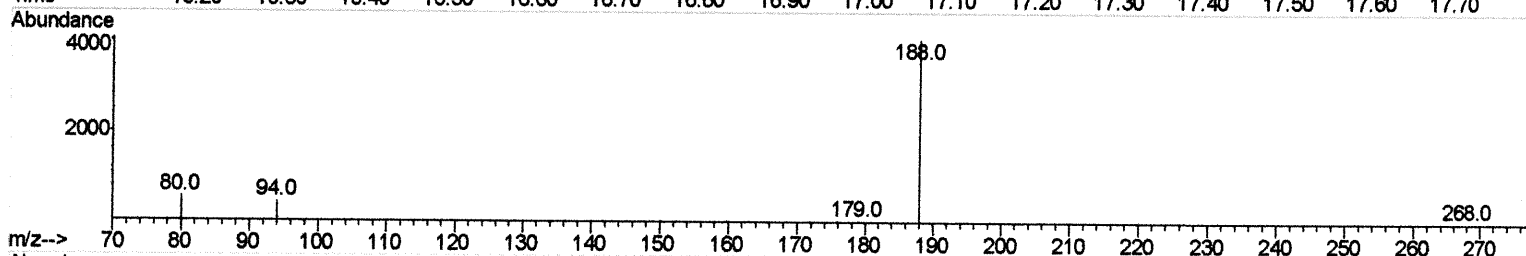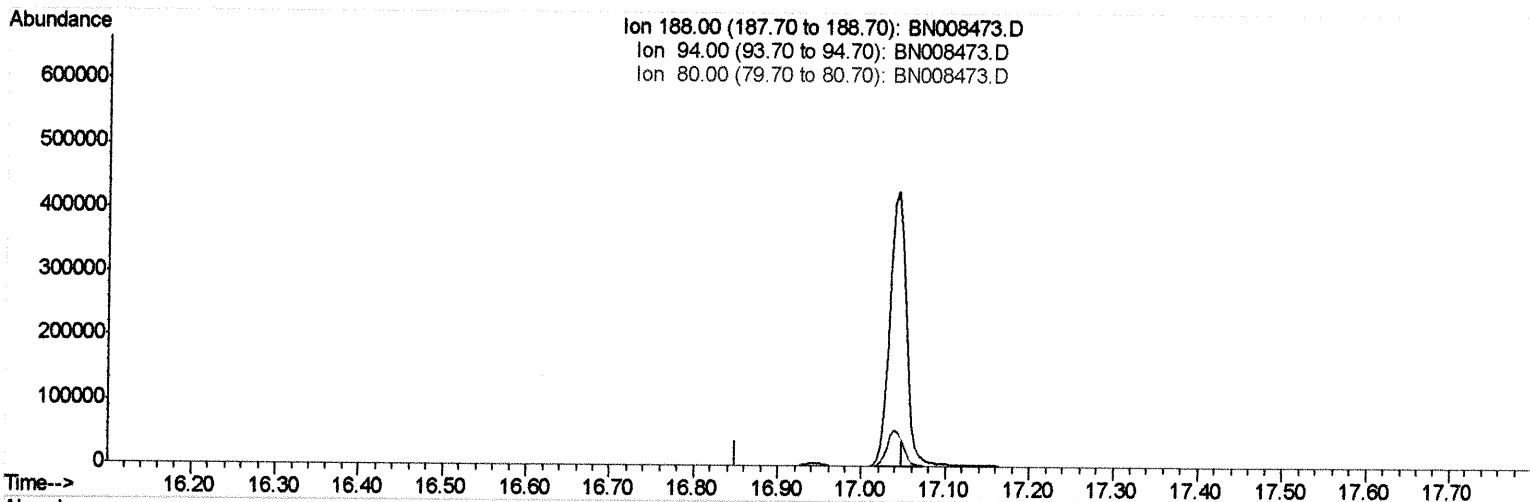

(10) Phenanthrene-d10 (I)

16.949min (-16.949) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	12.40	0.00#
80.00	15.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
 Data File : BN008473.D
 Acq On : 06 Nov 2019 18:58
 Operator : JU
 Sample : K5656-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5454

Manual Integrations
 APPROVED

Sohil
 11/8/2019 3:29:18 PM

Quant Time: Nov 07 12:25:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 12:16:36 2019
 Response via : Initial Calibration

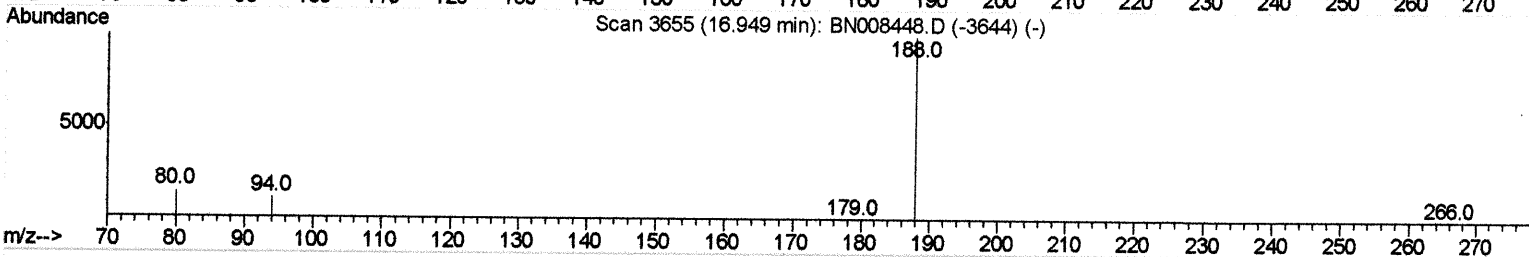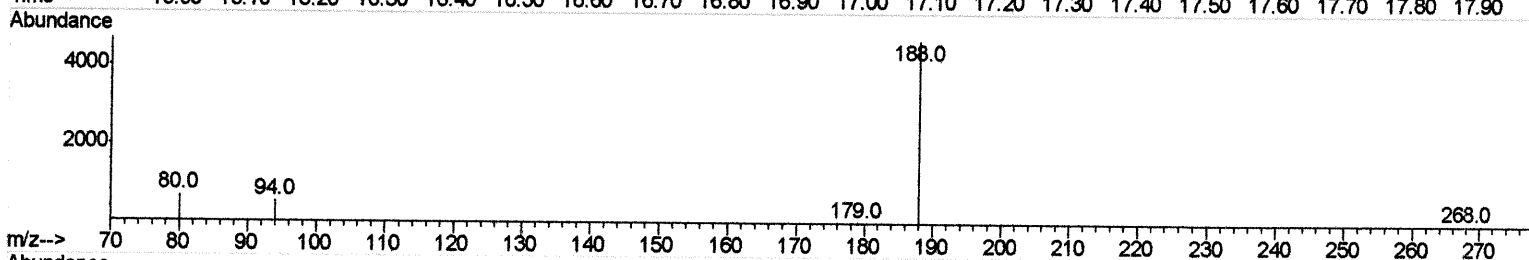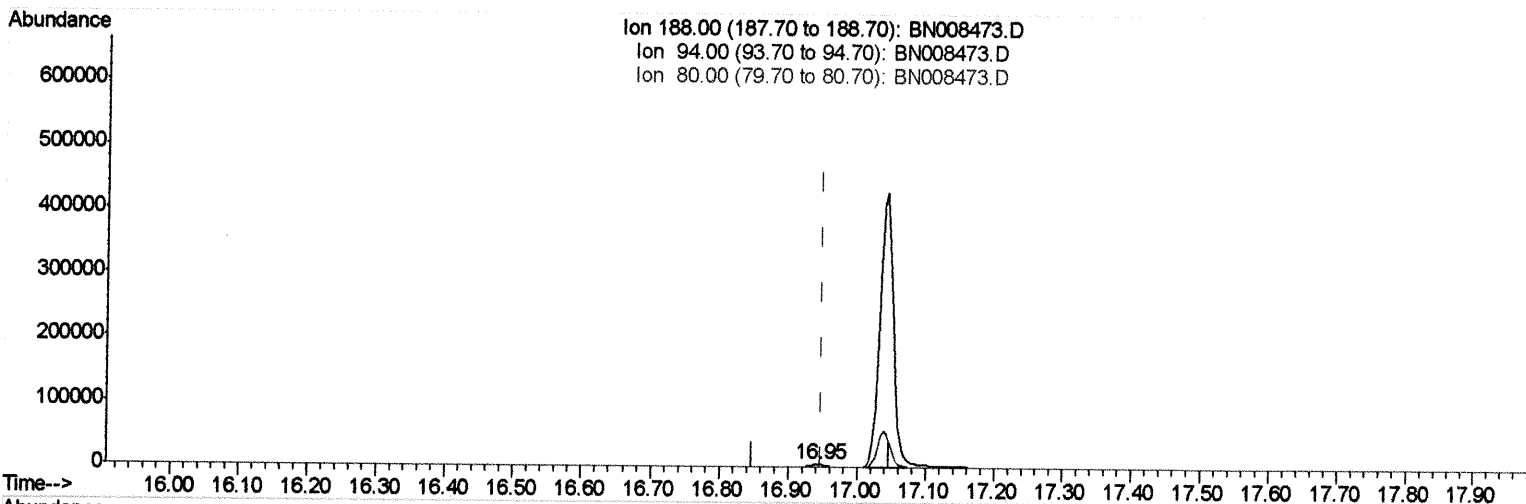

TIC: BN008473.D

(10) Phenanthrene-d10 (I)

16.945min (-0.004) 0.40ng/ul m

JU 11/8/19

response 6802

Ion	Exp%	Act%
188.00	100	100
94.00	12.40	11.67
80.00	15.50	14.60
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110619\
 Data File : BN008473.D
 Acq On : 06 Nov 2019 18:58
 Operator : JU
 Sample : K5656-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5454

Manual Integrations
 APPROVED

Sohil
 11/8/2019 3:29:18 PM

Quant Time: Nov 07 12:40:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 12:16:36 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	1248	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	5435	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	3256	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.95	188	6802m>	0.40	ng/ul>	0.00>
16) Chrysene-d12	21.16	240	5457	0.40	ng/ul	0.00
20) Perylene-d12	23.32	264	5302	0.40	ng/ul	-0.01

34 11/8/19

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.93	152	2178	0.25	ng/ul	0.02
14) Fluoranthene-d10	18.98	212	7185	0.35	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed