
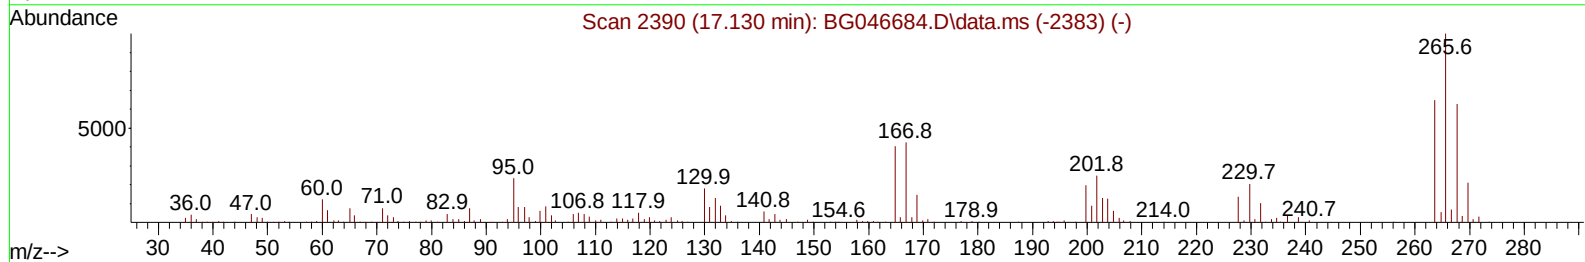
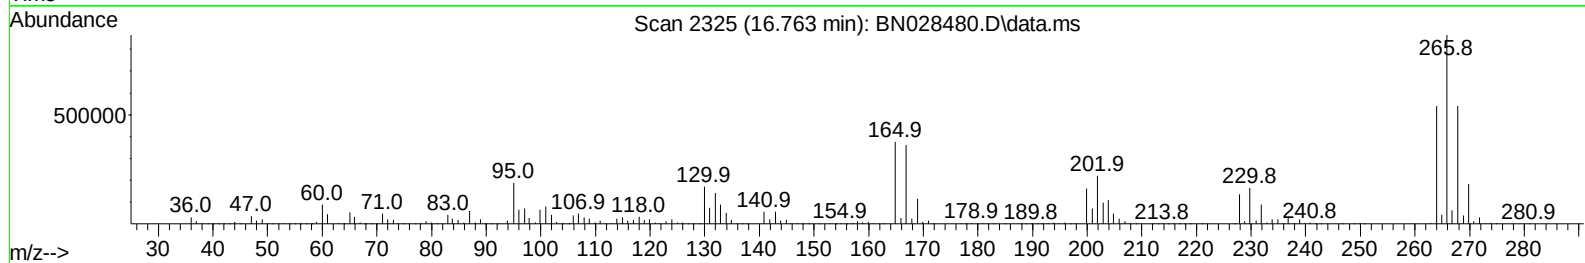


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110623\
Data File : BN028480.D
Acq On : 06 Nov 2023 13:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 04:32:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 04:32:06 2023
Response via : Initial Calibration

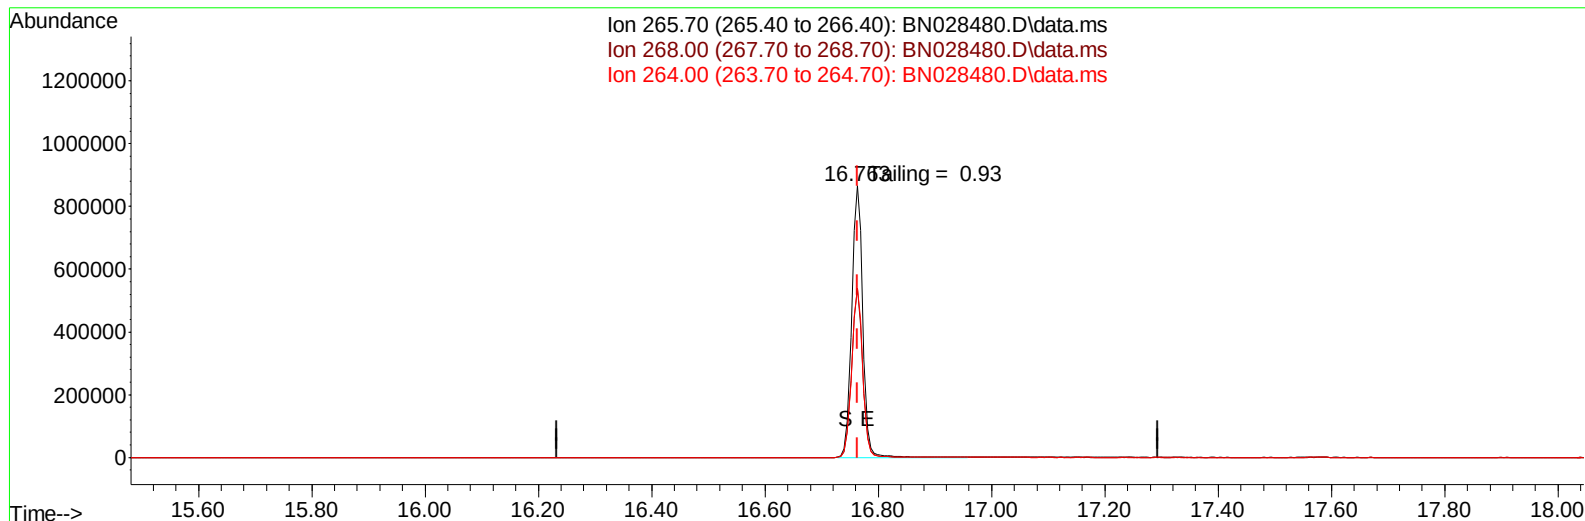




TIC: BN028480.D\data.ms

(70) Pentachlorophenol (C)**16.763min (0.000) 30201.46 ng****response 1182460**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.26
264.00	61.60	62.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110623\
Data File : BN028480.D
Acq On : 06 Nov 2023 13:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 04:32:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 04:32:06 2023
Response via : Initial Calibration

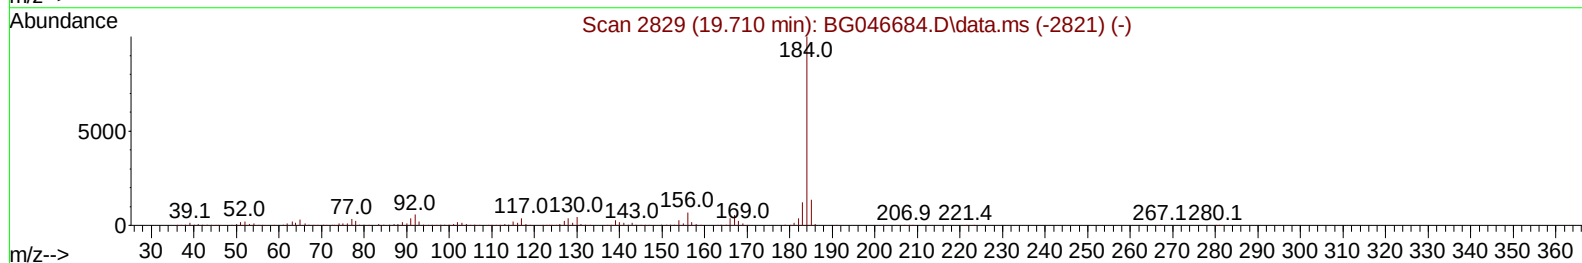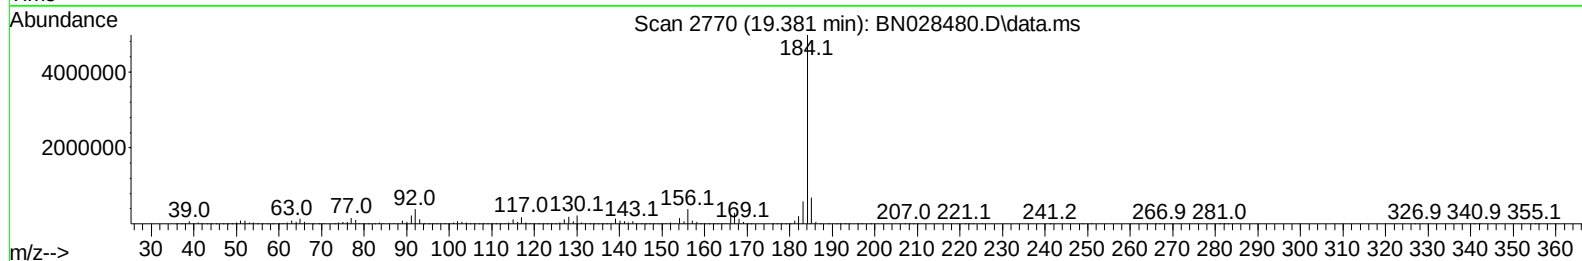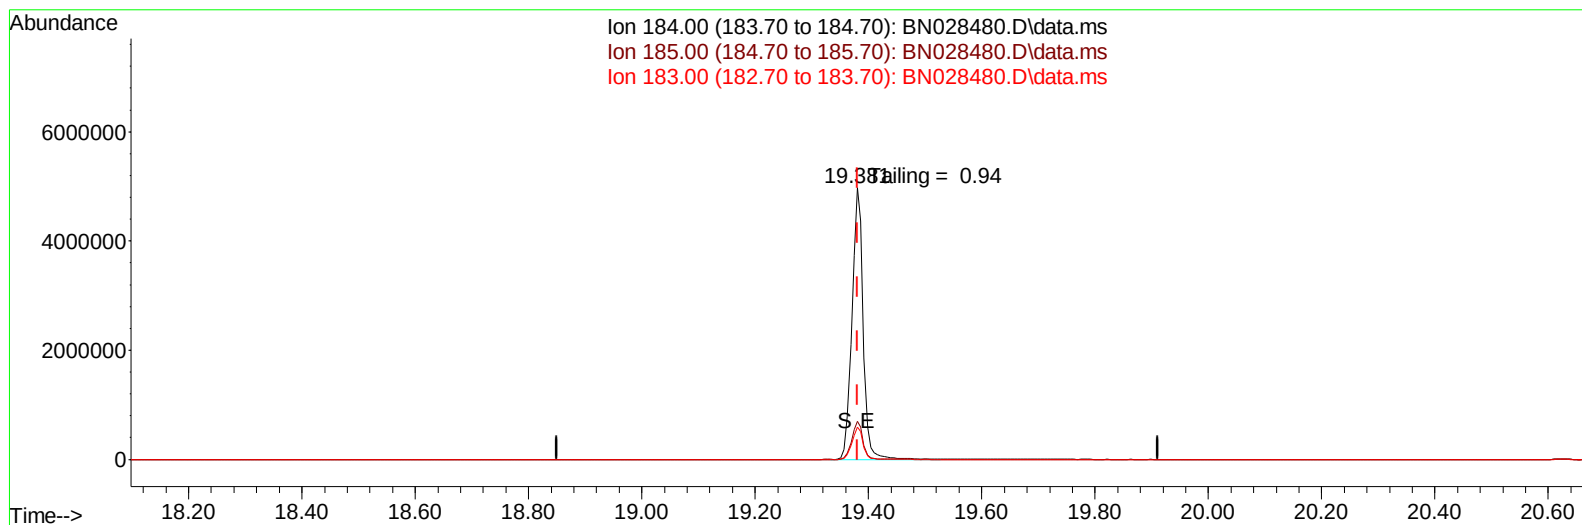

TIC: BN028480.D\data.ms

(77) Benzidine**19.381min (0.000) 652513.11 ng****response 6878974**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	12.02
0.00	0.00	0.00