


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110623\
Data File : BN028480.D
Acq On : 06 Nov 2023 13:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 02 06:26:50 2023

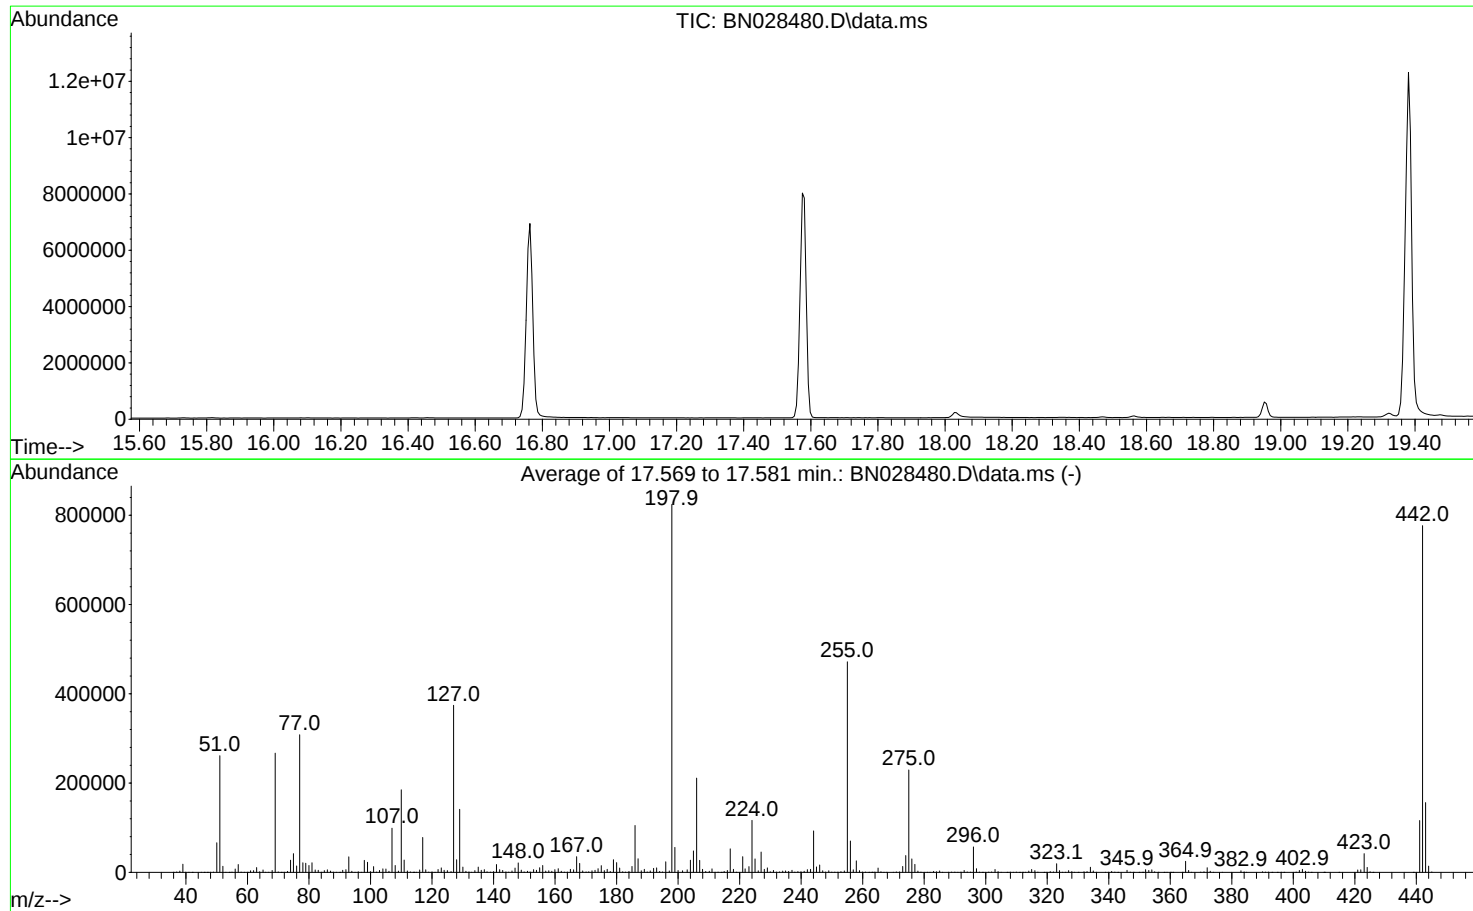




AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	31.7	261248	PASS
68	69	0.00	2	1.6	4306	PASS
69	198	0.00	100	32.4	266998	PASS
70	69	0.00	2	0.4	1171	PASS
127	198	10	80	45.4	374101	PASS
197	198	0.00	2	0.4	3395	PASS
198	198	100	100	100.0	824149	PASS
199	198	5	9	6.8	55981	PASS
275	198	10	60	27.8	229504	PASS
365	198	1	100	3.0	24590	PASS
441	198	0.01	100	14.1	116144	PASS
442	442	50	100	100.0	776768	PASS
443	442	15	24	20.1	156424	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110623\
Data File : BN028480.D
Acq On : 06 Nov 2023 13:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 07 04:32:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 04:32:06 2023
Response via : Initial Calibration

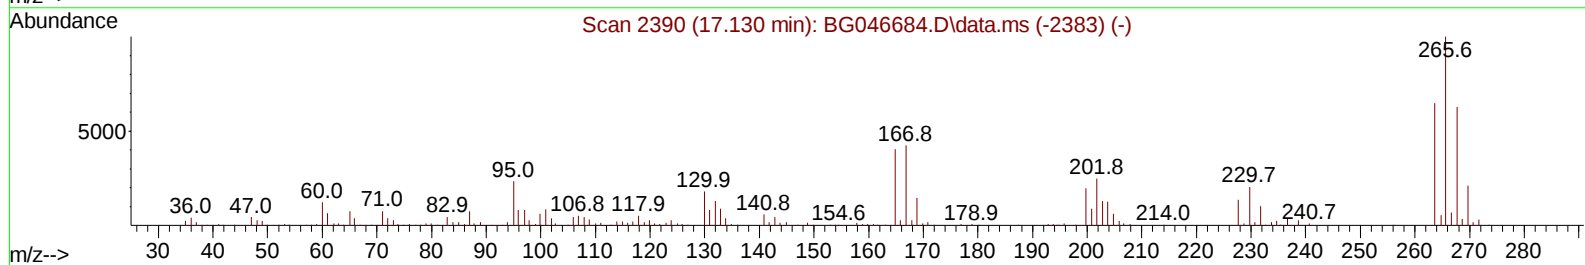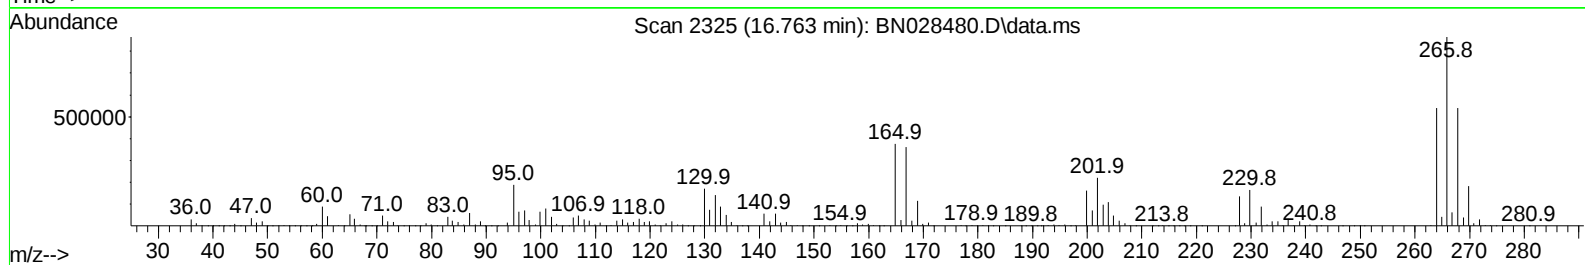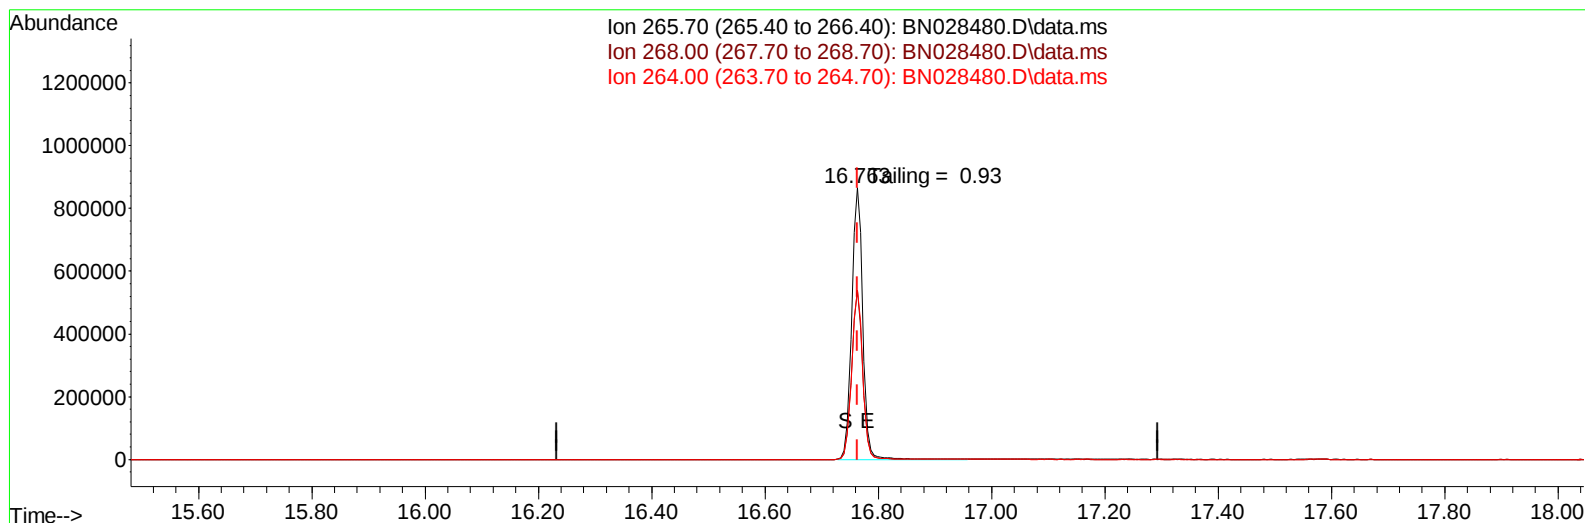

TIC: BN028480.D\data.ms

(70) Pentachlorophenol (C)

16.763min (0.000) 30201.46 ng




response 1182460

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.26
264.00	61.60	62.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110623\
Data File : BN028480.D
Acq On : 06 Nov 2023 13:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 07 04:32:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 04:32:06 2023
Response via : Initial Calibration

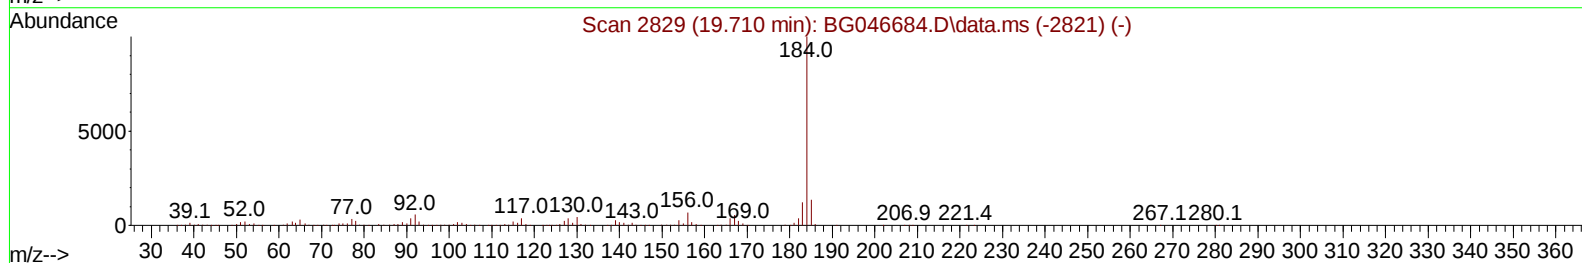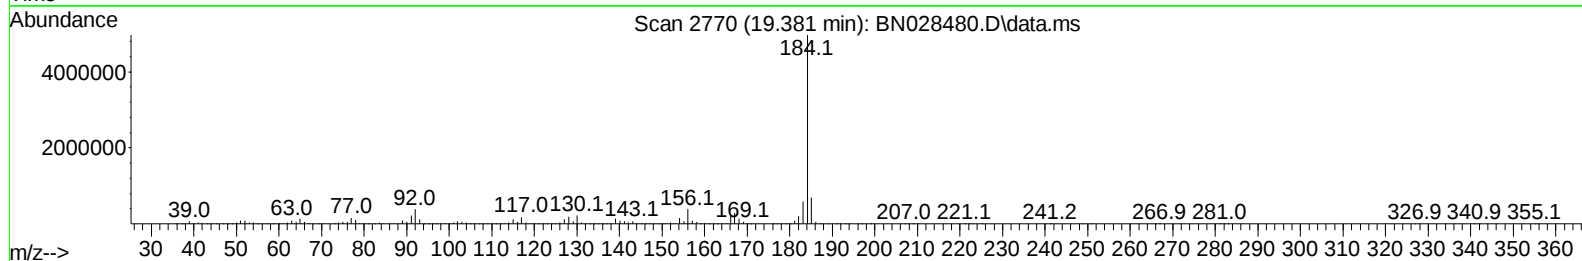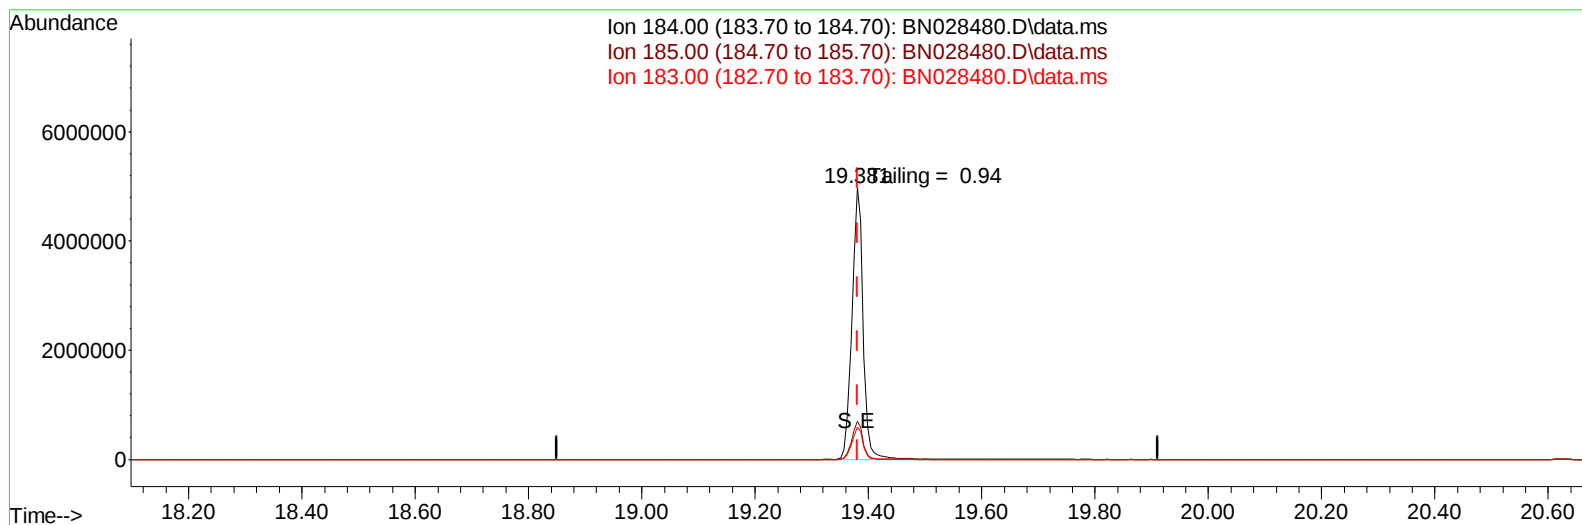

TIC: BN028480.D\data.ms

(77) Benzidine

19.381min (0.000) 652513.11 ng

response 6878974

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/6/2023	BNA_N	<u>BN028480.D</u>
Compound Name	Response	Retention Time
DDT	3278650	20.628
DDD	32492	20.233
DDE	1916	19.669
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
34408	3313058	1.04

Instrument :
BNA_N
ClientSampleId :
DFTPP