

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110718\
 Data File : BN003456.D
 Acq On : 07 Nov 2018 17:45
 Operator : MJ/SJ
 Sample : J5829-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Nov 08 14:32:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN102418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 07 08:25:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	95044	20.00	ng	0.00
21) Naphthalene-d8	10.65	136	429554	20.00	ng	0.00
39) Acenaphthene-d10	14.49	164	260799	20.00	ng	0.00
64) Phenanthrene-d10	17.23	188	576225	20.00	ng	0.00
76) Chrysene-d12	21.40	240	455809	20.00	ng	0.00
87) Perylene-d12	23.72	264	437362	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.41	112	223339	40.93	ng	0.00
7) Phenol-d6	7.00	99	179050	23.08	ng	-0.01
23) Nitrobenzene-d5	9.02	82	666387	88.97	ng	0.00
42) 2,4,6-Tribromophenol	15.97	330	359427	102.35	ng	0.00
45) 2-Fluorobiphenyl	13.11	172	1859850	96.73	ng	0.00
79) Terphenyl-d14	19.85	244	2261600	106.11	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.03	88	10429	4.025	ng	# 1
10) Phenol	7.03	94	22737	2.777	ng	95
19) n-Nitroso-di-n-propylamine	9.02	70	84779	15.152	ng	# 75
51) 2,6-Dinitrotoluene	14.49	165	33262	6.950	ng	# 28
57) 2,4-Dinitrotoluene	14.49	165	33262	5.126	ng	# 19
67) 4-Bromophenyl-phenylether	15.97	248	22984	3.542	ng	# 1
77) Benzidine	19.85	184	27381	2.052	ng	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110718\
Data File : BN003456.D
Acq On : 07 Nov 2018 17:45
Operator : MJ/SJ
Sample : J5829-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Nov 08 14:32:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN102418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 07 08:25:32 2018
Response via : Initial Calibration

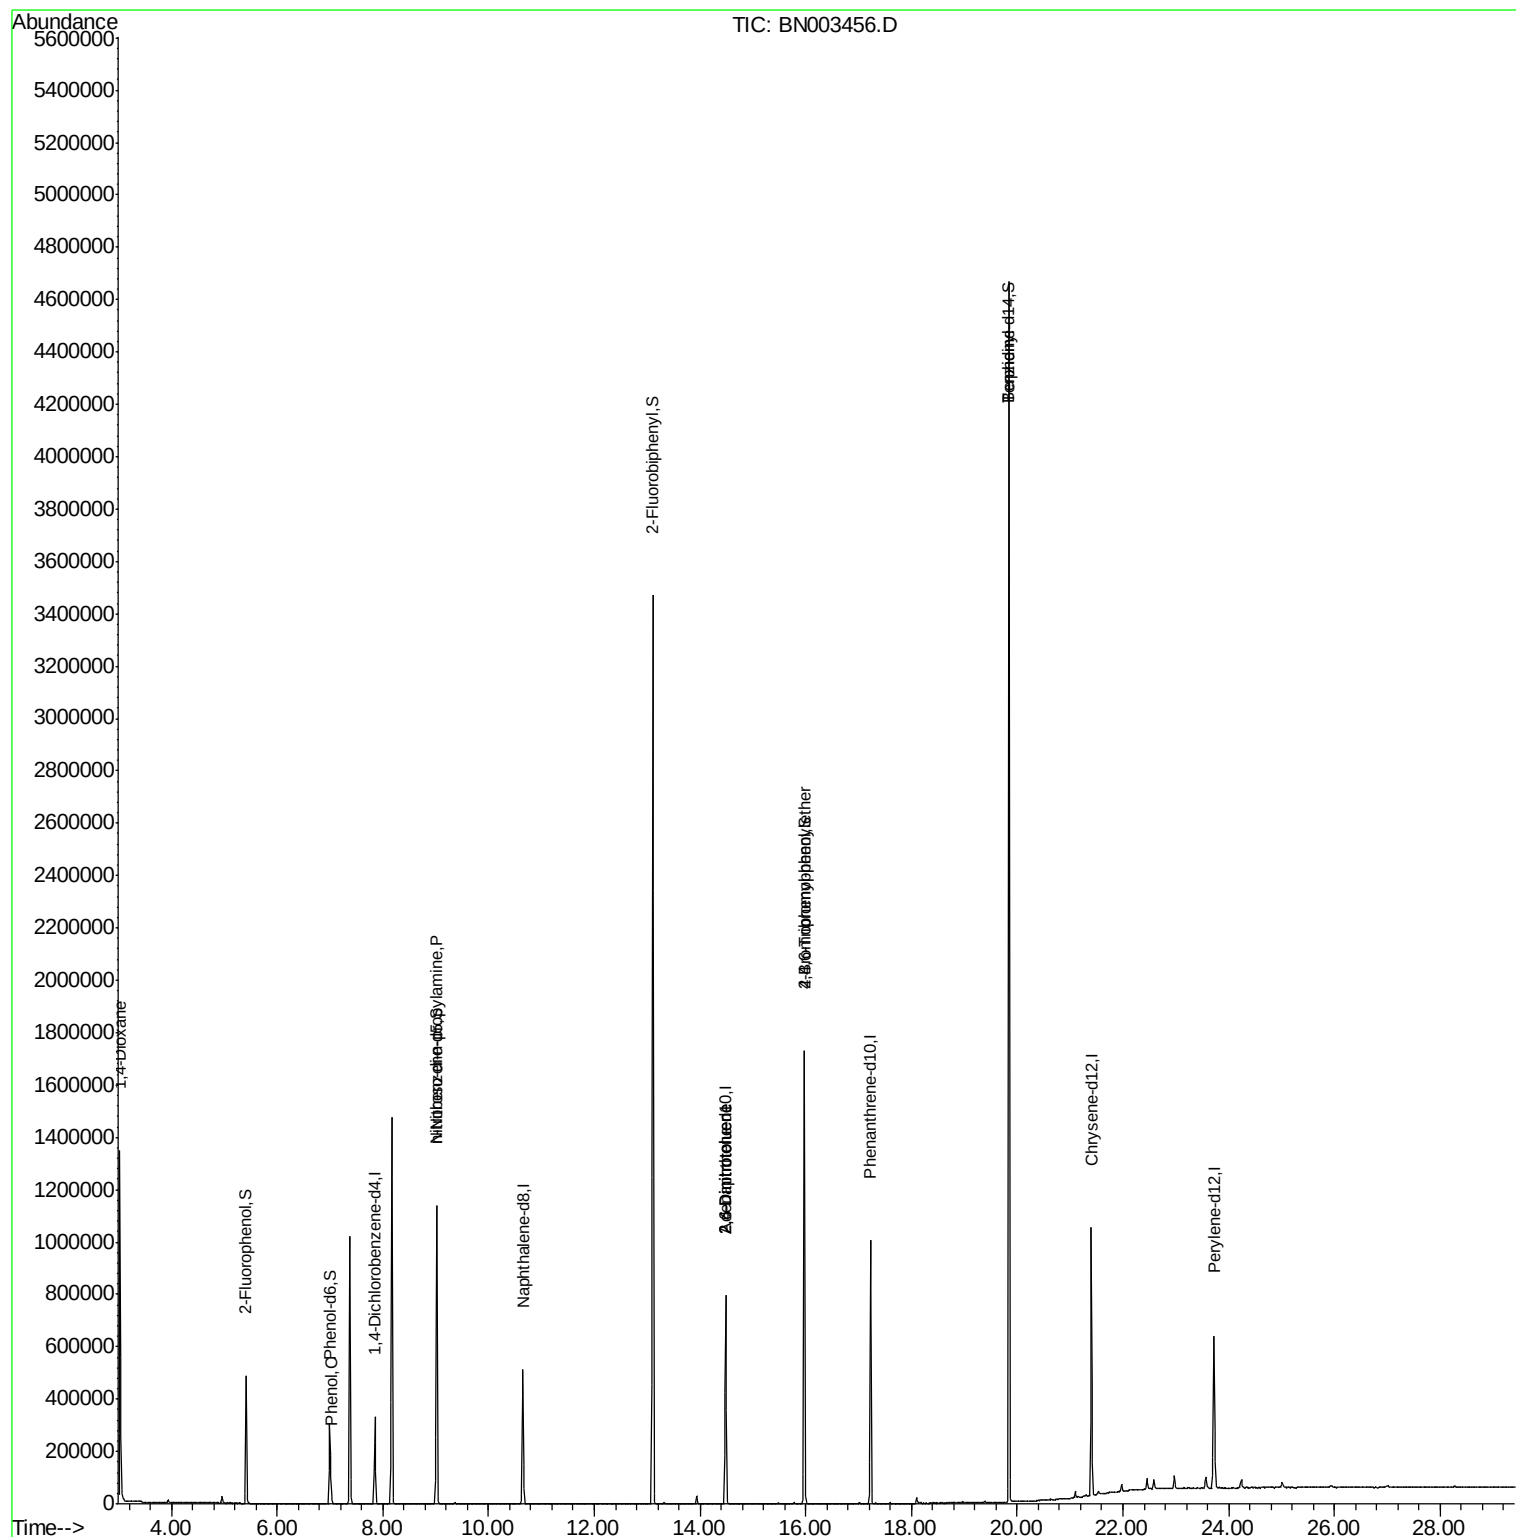

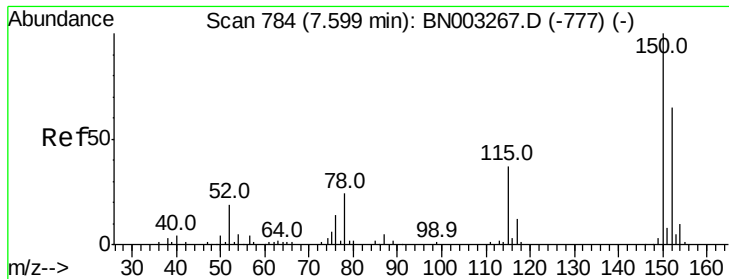


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.85 min Scan# 827
Delta R.T. 0.00 min
Lab File: BN003456.D
Acq: 07 Nov 2018 17:45

Instrument :
BNA_N
ClientSampleId :

Tot Ion:152 Resp: 95044
Ion Ratio Lower Upper
152 100
150 158.3 123.8 185.8
115 55.6 45.9 68.9

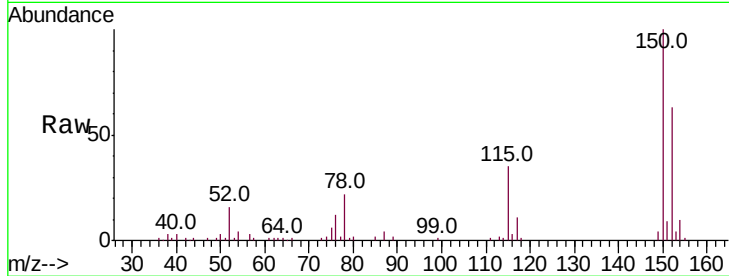


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

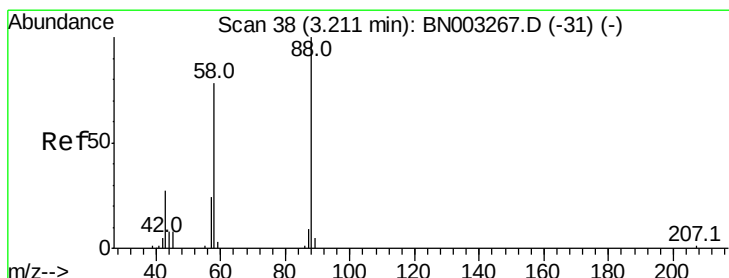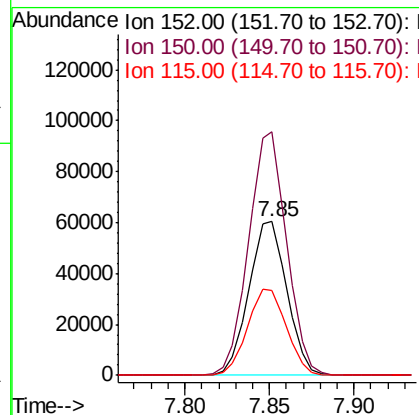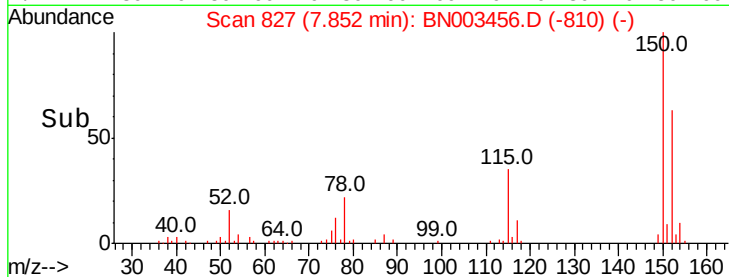



#2


1,4-Dioxane
Concen: 4.025 ng
RT: 3.03 min Scan# 7
Delta R.T. -0.31 min
Lab File: BN003456.D
Acq: 07 Nov 2018 17:45

Tgt Ion: 88 Resp: 10429
Ion Ratio Lower Upper
88 100
58 25.1 61.1 91.7#
43 2148.3 22.2 33.4#

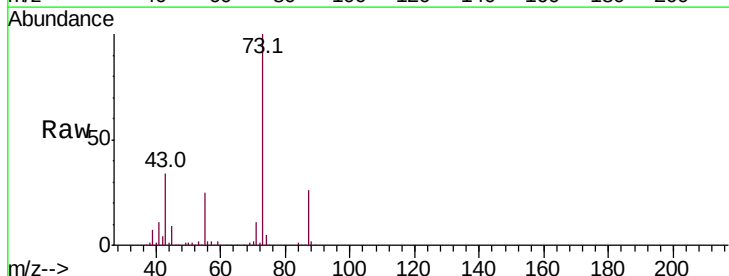

Abundance Ion 88.00 (87.70 to 88.70): BNC
Ion 58.00 (57.70 to 58.70): BNC
Ion 43.00 (42.70 to 43.70): BNC

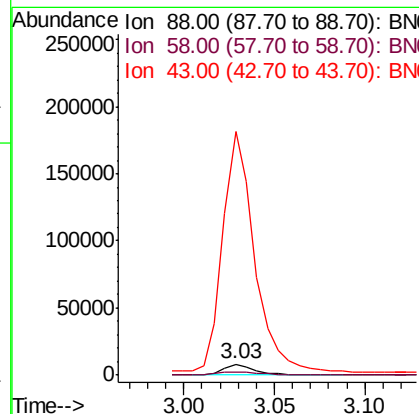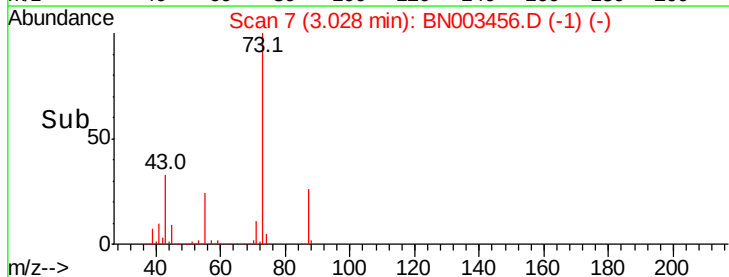

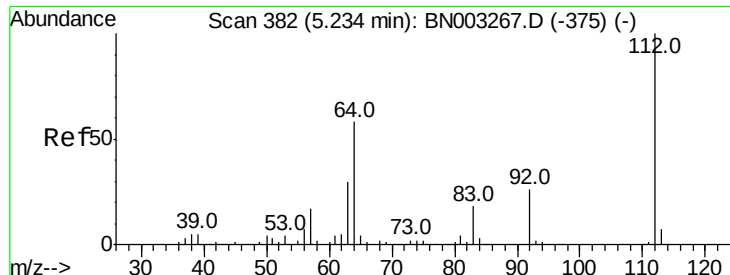

#5

2-Fluorophenol

Concen: 40.928 ng

RT: 5.41 min Scan# 412


Delta R.T. 0.00 min

Lab File: BN003456.D




Acq: 07 Nov 2018 17:45

Instrument :
BNA_N
ClientSampled :

Tot Ion:	112	Resp:	223339
Ion	Ratio	Lower	Upper
112	100		
64	53.1	46.6	69.8
63	26.9	23.8	35.8

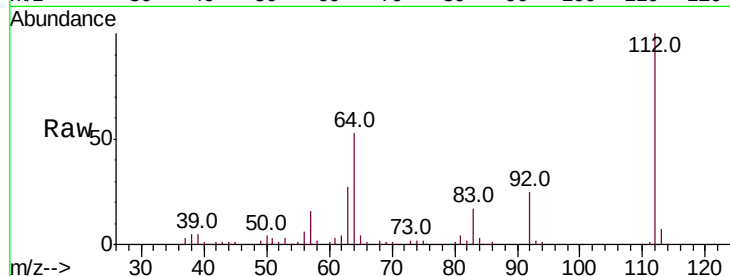

Abundance Ion 112.00 (111.70 to 112.70): BNC
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

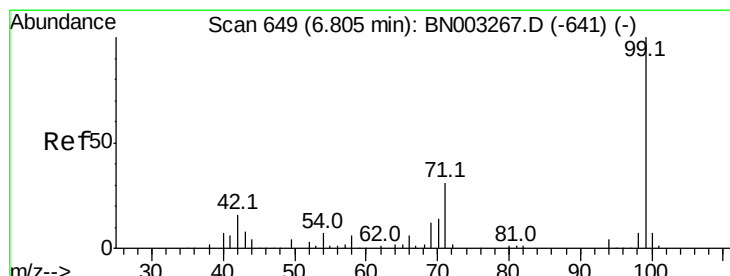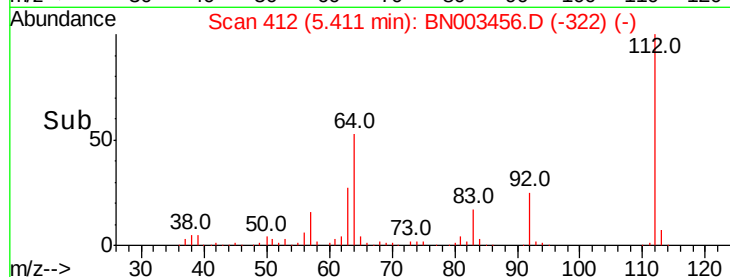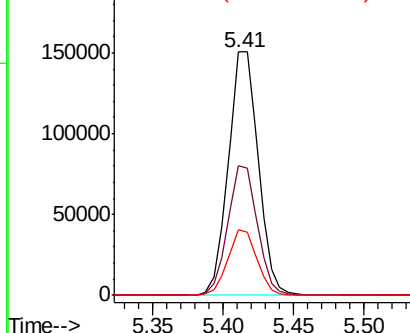

#7

Phenol-d6

Concen: 23.075 ng


RT: 7.00 min Scan# 682

Delta R.T. -0.01 min



Lab File: BN003456.D


Acq: 07 Nov 2018 17:45

Tgt Ion:	99	Resp:	179050
Ion	Ratio	Lower	Upper
99	100		
42	15.0	13.0	19.6
71	29.8	24.5	36.7

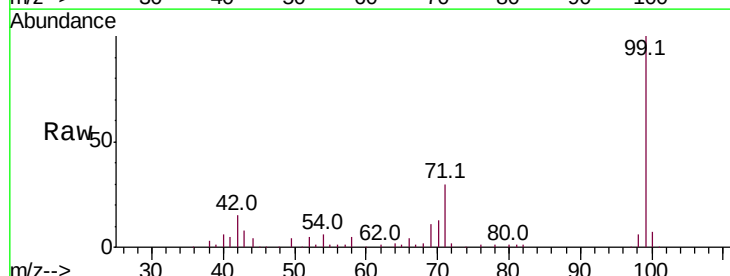

Abundance Ion 99.00 (98.70 to 99.70): BNC
Ion 42.00 (41.70 to 42.70): BNC
Ion 71.00 (70.70 to 71.70): BNC

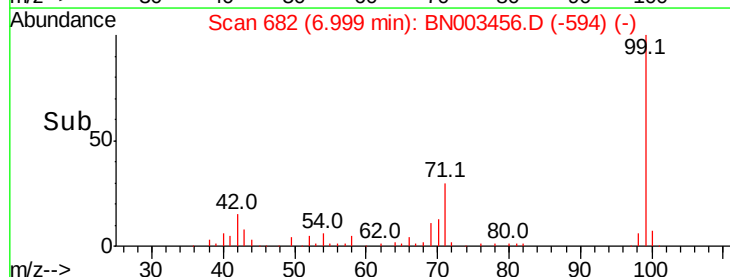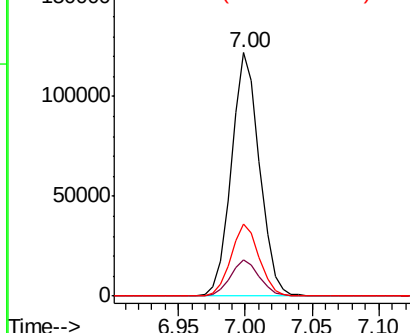







#10
Phenol
Concen: 2.777 ng
RT: 7.03 min Scan# 687
Delta R.T. -0.01 min
Lab File: BN003456.D
Acq: 07 Nov 2018 17:45

Instrument :
BNA_N
ClientSampleId :

Tot Ion: 94 Resp: 22737
Ion Ratio Lower Upper
94 100
65 26.0 7.7 47.7
66 32.1 15.8 55.8

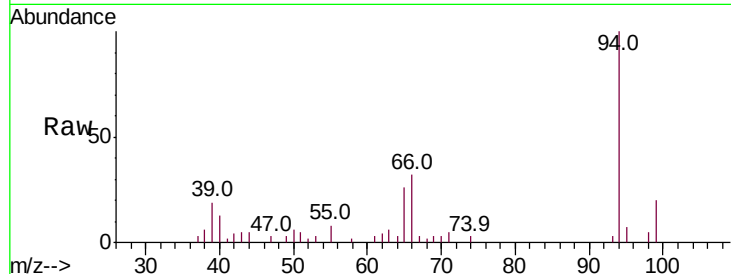


Abundance Ion 94.00 (93.70 to 94.70): BN0
Ion 65.00 (64.70 to 65.70): BN0
Ion 66.00 (65.70 to 66.70): BN0

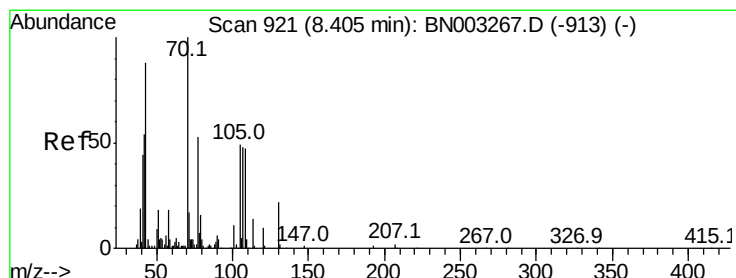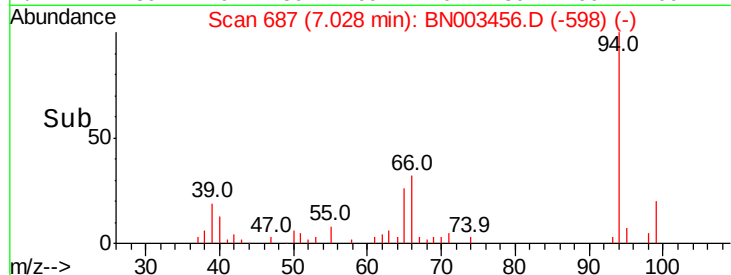
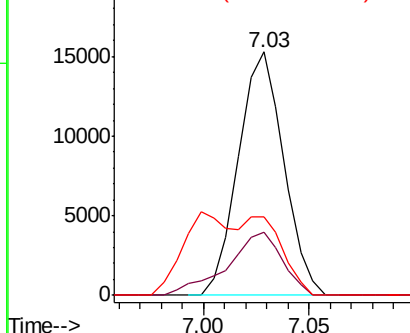



#19
n-Nitroso-di-n-propylamine
Concen: 15.152 ng
RT: 9.02 min Scan# 1025
Delta R.T. 0.36 min
Lab File: BN003456.D
Acq: 07 Nov 2018 17:45

Tgt Ion: 70 Resp: 84779
Ion Ratio Lower Upper
70 100
42 42.0 43.5 65.3#
101 0.0 8.6 12.8#
130 2.4 18.0 27.0#

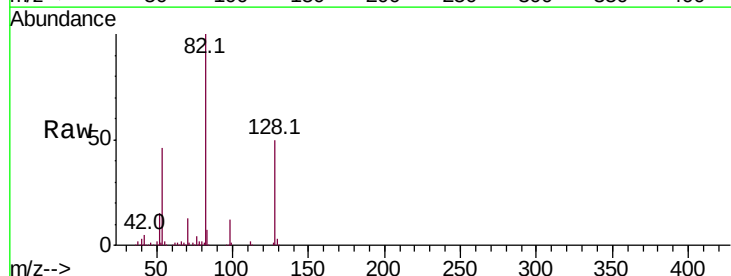

Abundance Ion 70.00 (69.70 to 70.70): BN0
Ion 42.00 (41.70 to 42.70): BN0
Ion 101.00 (100.70 to 101.70): BN0
Ion 130.00 (129.70 to 130.70): BN0

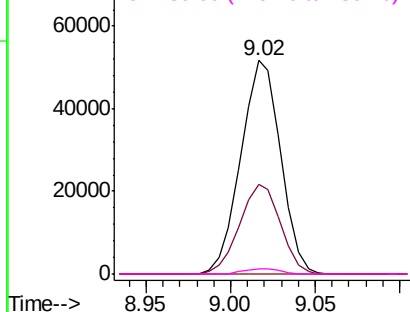


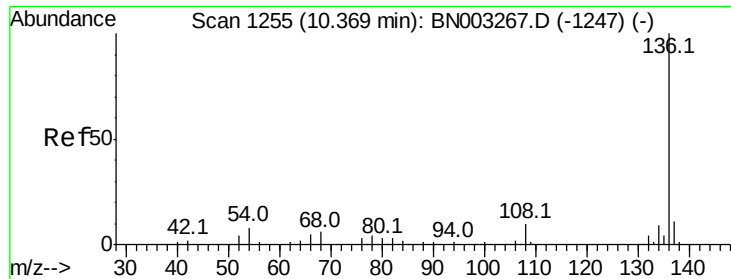




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.65 min Scan# 1302
Delta R.T. -0.01 min
Lab File: BN003456.D
Acq: 07 Nov 2018 17:45

Instrument :
BNA_N
ClientSampleId :

Tot Ion:136	Resp:	429554
Ion Ratio	Lower	Upper
136	100	
137	11.2	8.7 13.1
54	7.3	6.6 10.0
68	6.0	4.6 7.0

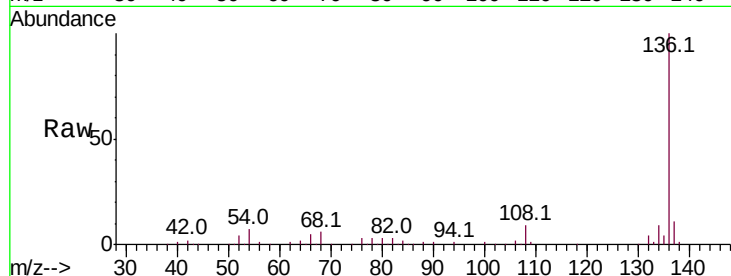


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BNC
Ion 68.00 (67.70 to 68.70): BNC

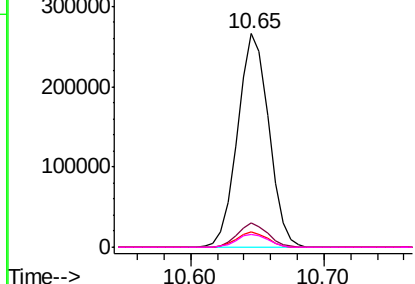




#23
Nitrobenzene-d5
Concen: 88.969 ng
RT: 9.02 min Scan# 1025
Delta R.T. -0.01 min
Lab File: BN003456.D
Acq: 07 Nov 2018 17:45

Tgt Ion: 82	Resp:	666387
Ion Ratio	Lower	Upper
82	100	
128	50.0	37.1 55.7
54	45.5	39.4 59.2



Abundance Ion 82.00 (81.70 to 82.70): BNC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BNC

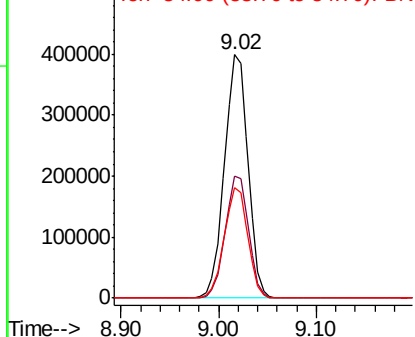

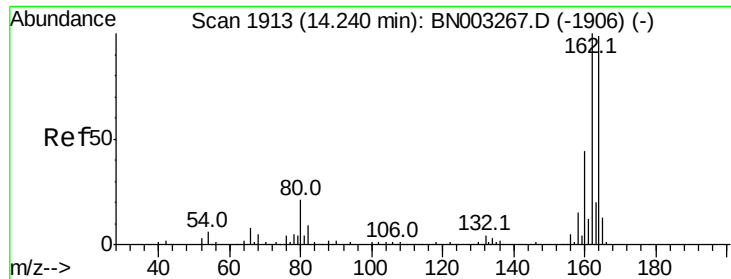

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.49 min Scan# 1955

Delta R.T. 0.00 min

Lab File: BN003456.D

Acq: 07 Nov 2018 17:45

Instrument :

BNA_N

ClientSampleId :


Tot Ion:164 Resp: 260799

Ion Ratio Lower Upper

164 100

162 101.4 80.8 121.2




160 44.8 35.5 53.3



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

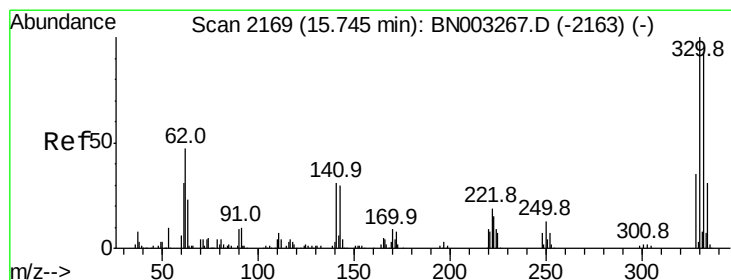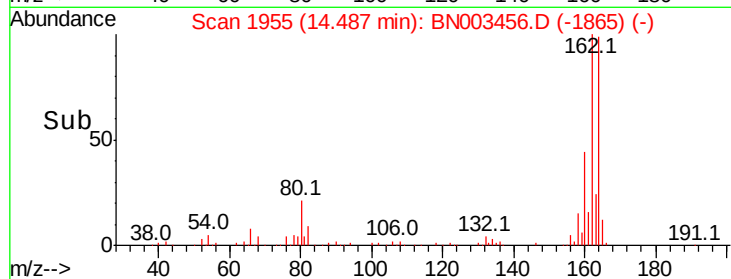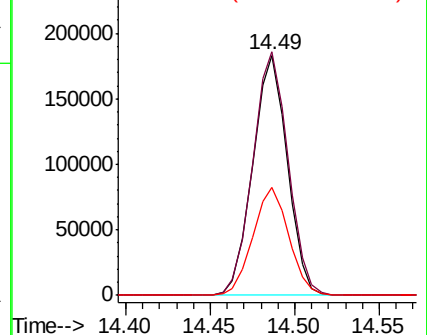

#42

2,4,6-Tribromophenol

Concen: 102.350 ng

RT: 15.97 min Scan# 2208

Delta R.T. -0.01 min

Lab File: BN003456.D

Acq: 07 Nov 2018 17:45


Tgt Ion:330 Resp: 359427

Ion Ratio Lower Upper

330 100

332 96.2 76.6 114.8



141 27.5 24.5 36.7

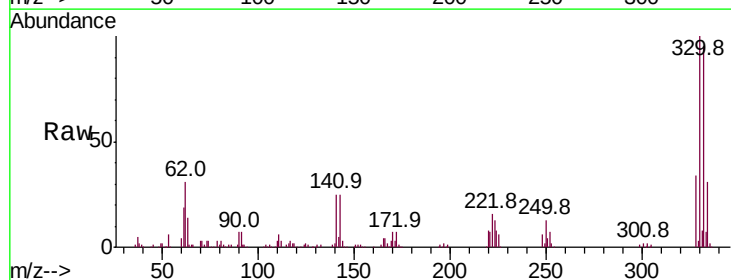


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

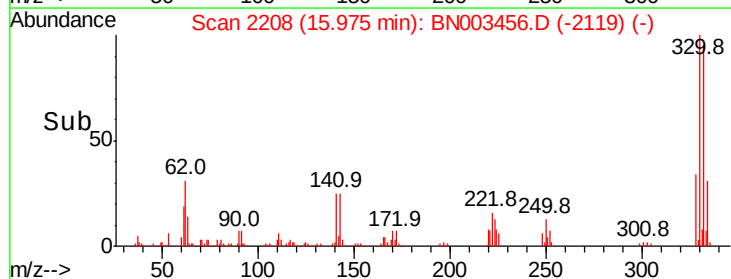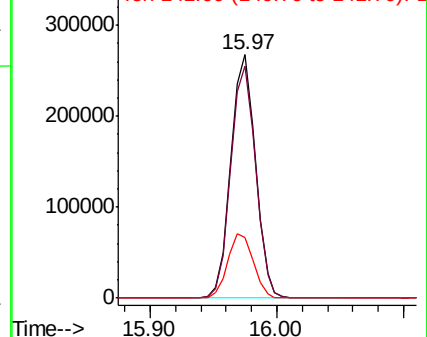







#45
 2-Fluorobiphenyl
 Concen: 96.731 ng
 RT: 13.11 min Scan# 1721
 Delta R.T. 0.00 min
 Lab File: BN003456.D
 Acq: 07 Nov 2018 17:45

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:172 Resp: 1859850




Ion	Ratio	Lower	Upper
172	100		
171	36.5	28.2	42.4
170	23.7	18.4	27.6

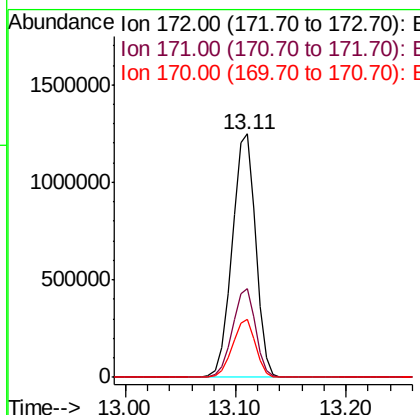


#51
 2,6-Dinitrotoluene
 Concen: 6.950 ng
 RT: 14.49 min Scan# 1955
 Delta R.T. 0.41 min
 Lab File: BN003456.D
 Acq: 07 Nov 2018 17:45

Tgt Ion:165 Resp: 33262

Ion	Ratio	Lower	Upper
165	100		
63	0.0	39.2	58.8#
89	0.0	38.9	58.3#

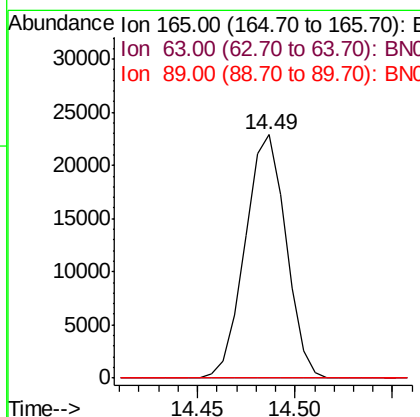


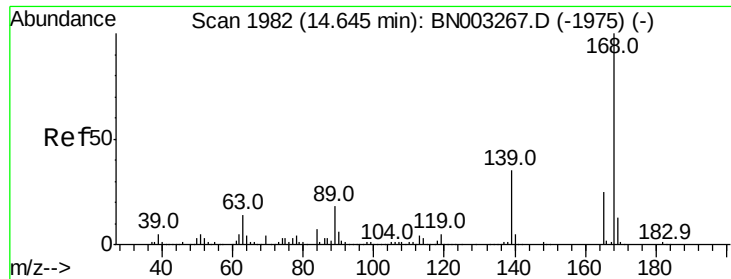




#57
 2,4-Dinitrotoluene
 Concen: 5.126 ng
 RT: 14.49 min Scan# 1955
 Delta R.T. -0.37 min
 Lab File: BN003456.D
 Acq: 07 Nov 2018 17:45

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:165 Resp: 33262
 Ion Ratio Lower Upper
 165 100
 63 0.0 45.8 68.6#
 89 0.0 58.7 88.1#
 182 0.0 2.3 3.5#




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BNC
 Ion 89.00 (88.70 to 89.70): BNC
 Ion 182.00 (181.70 to 182.70): E

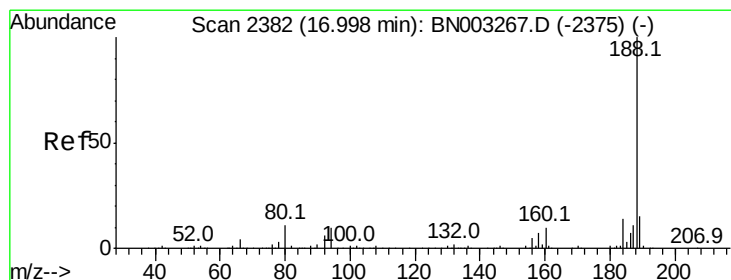
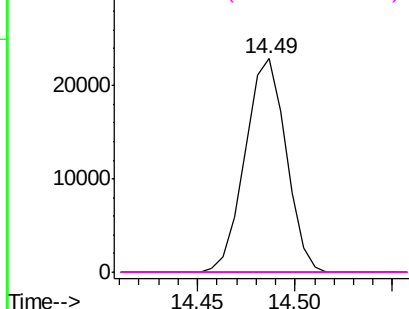



#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.23 min Scan# 2421
 Delta R.T. -0.01 min
 Lab File: BN003456.D
 Acq: 07 Nov 2018 17:45

Tgt Ion:188 Resp: 576225
 Ion Ratio Lower Upper
 188 100
 94 9.6 8.1 12.1
 80 10.6 8.6 13.0

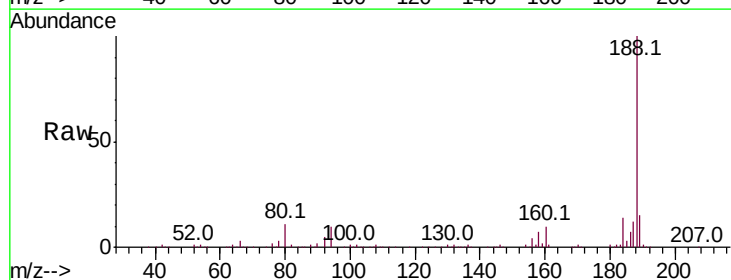

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BNC
 Ion 80.00 (79.70 to 80.70): BNC

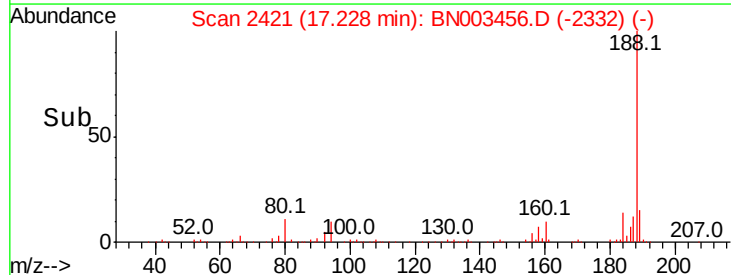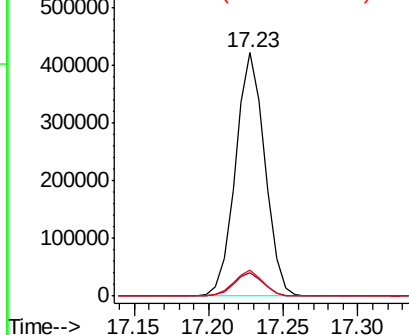


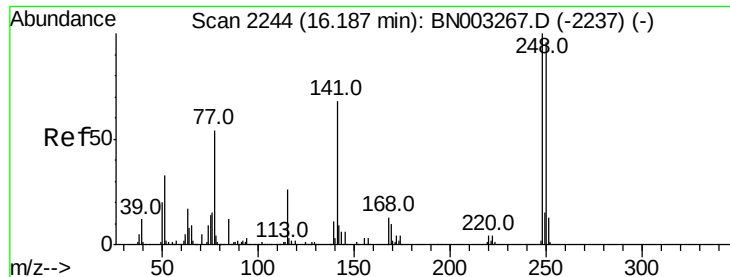




#67
4-Bromophenyl-phenylether
Concen: 3.542 ng
RT: 15.97 min Scan# 2208
Delta R.T. -0.45 min
Lab File: BN003456.D
Acq: 07 Nov 2018 17:45

Instrument :
BNA_N
ClientSampleId :

Tot Ion:248 Resp: 22984
Ion Ratio Lower Upper
248 100
250 201.8 76.4 114.6#
141 401.4 54.2 81.4#

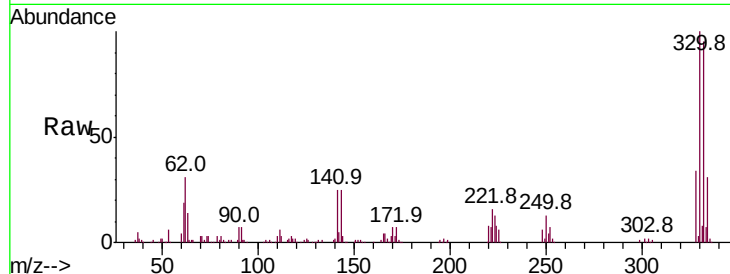


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

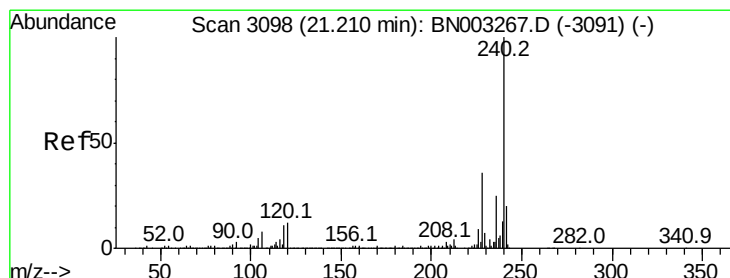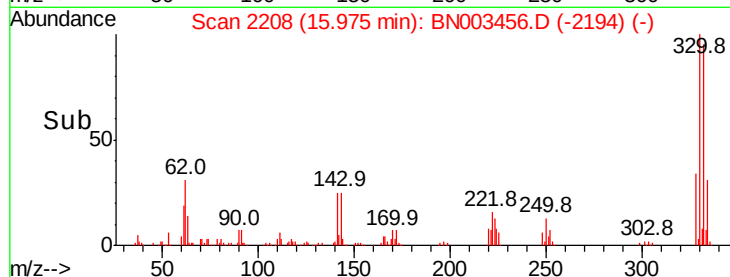
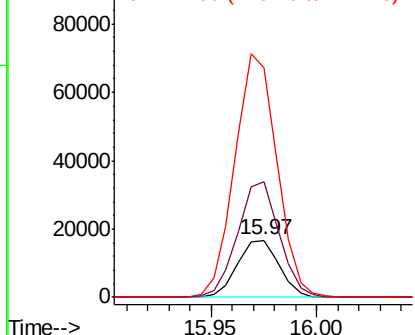



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.40 min Scan# 3131
Delta R.T. -0.01 min
Lab File: BN003456.D
Acq: 07 Nov 2018 17:45

Tgt Ion:240 Resp: 455809
Ion Ratio Lower Upper
240 100
120 11.7 9.4 14.0
236 25.7 20.3 30.5

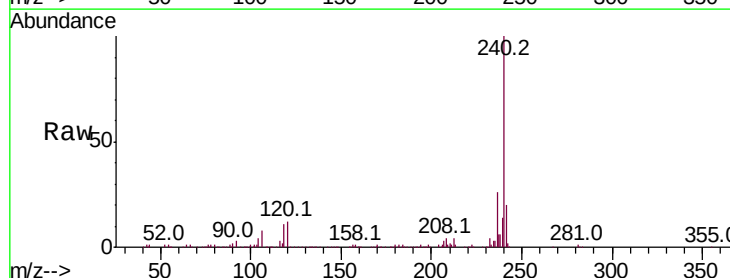

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

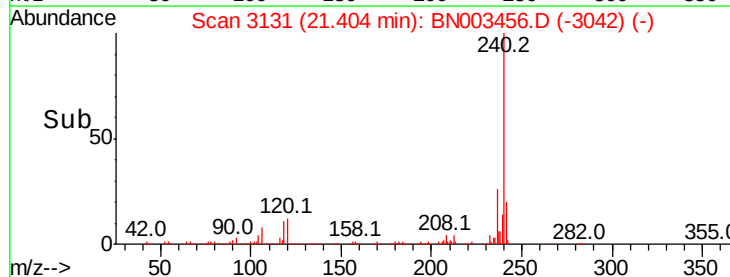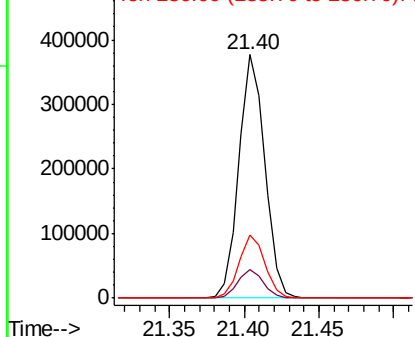



#77

Benzidine

Concen: 2.052 ng

RT: 19.85 min Scan# 2866

Delta R.T. 0.37 min

Lab File: BN003456.D

Acq: 07 Nov 2018 17:45

Instrument :

BNA_N

ClientSampled :


Tot Ion:184 Resp: 27381

Ion Ratio Lower Upper

184 100

185 15.7 11.5 17.3




183 8.3 9.4 14.0#



Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

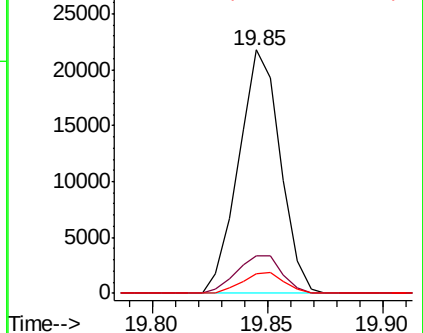

#79

Terphenyl-d14

Concen: 106.109 ng

RT: 19.85 min Scan# 2866

Delta R.T. -0.01 min

Lab File: BN003456.D

Acq: 07 Nov 2018 17:45


Tgt Ion:244 Resp: 2261600

Ion Ratio Lower Upper

244 100

212 6.7 5.4 8.0



122 11.3 9.4 14.2




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

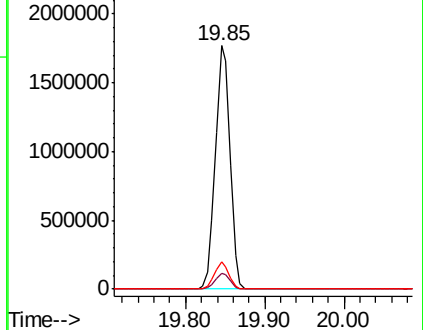


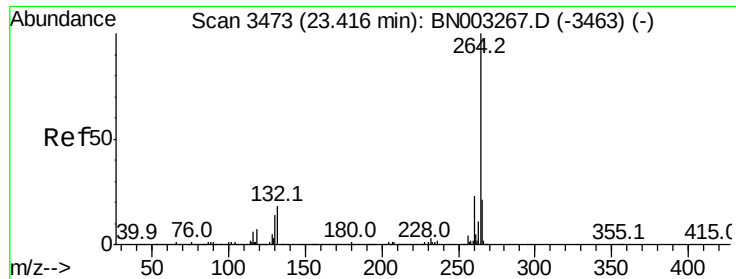

#87
Pervlene-d12
Concen: 20.000 ng
RT: 23.72 min Scan# 3525
Delta R.T. -0.01 min
Lab File: BN003456.D
Acq: 07 Nov 2018 17:45

Instrument :
BNA_N
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.4	18.5	27.7
265	21.7	16.6	25.0

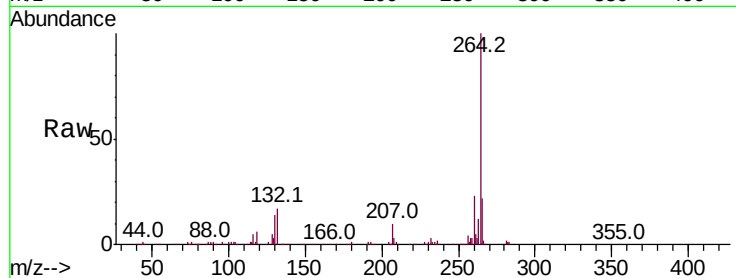

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

