


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110718\
 Data File : BN003450.D
 Acq On : 07 Nov 2018 14:15
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN102418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 07 08:25:32 2018

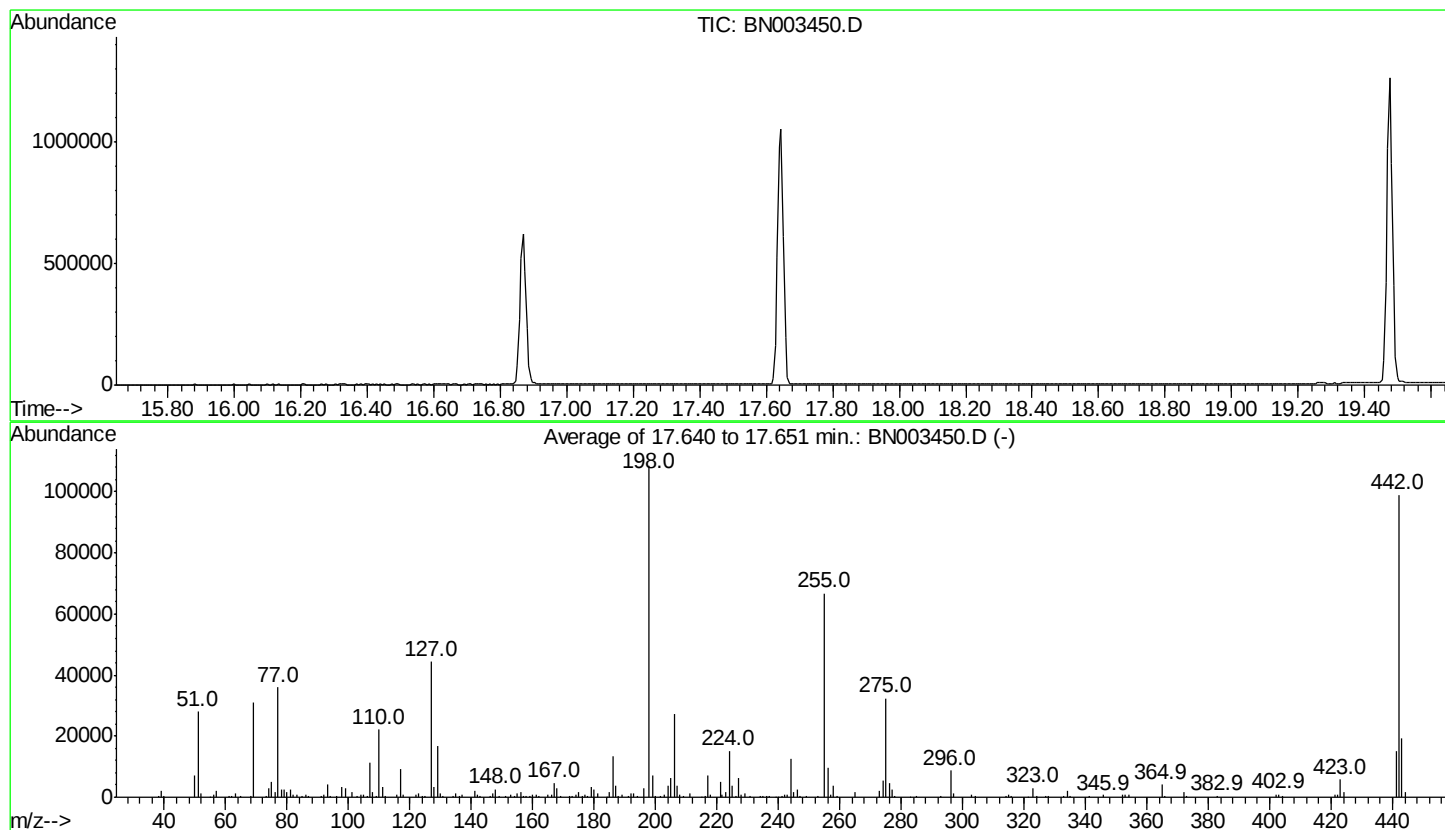

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.8	27987	PASS
68	69	0.00	2	1.9	606	PASS
69	198	0.00	100	28.7	31213	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.8	44298	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	108584	PASS
199	198	5	9	6.6	7137	PASS
275	198	10	60	29.9	32482	PASS
365	198	1	100	3.8	4118	PASS
441	198	0.01	100	14.0	15246	PASS
442	198	50	100	91.3	99106	PASS
443	442	15	24	19.6	19400	PASS