

Data File : BN008485.D

Acq On : 07 Nov 2019 15:14

Operator : JU

Sample : K5565-01

Misc :

ALS Vial : 8 Sample Multiplier: 1




Quant Time: Nov 08 05:45:39 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Nov 08 05:42:36 2019

Response via : Initial Calibration

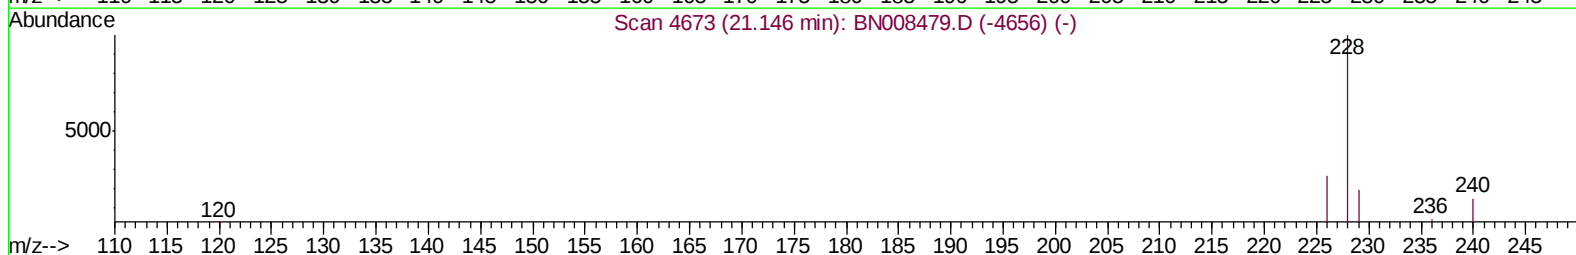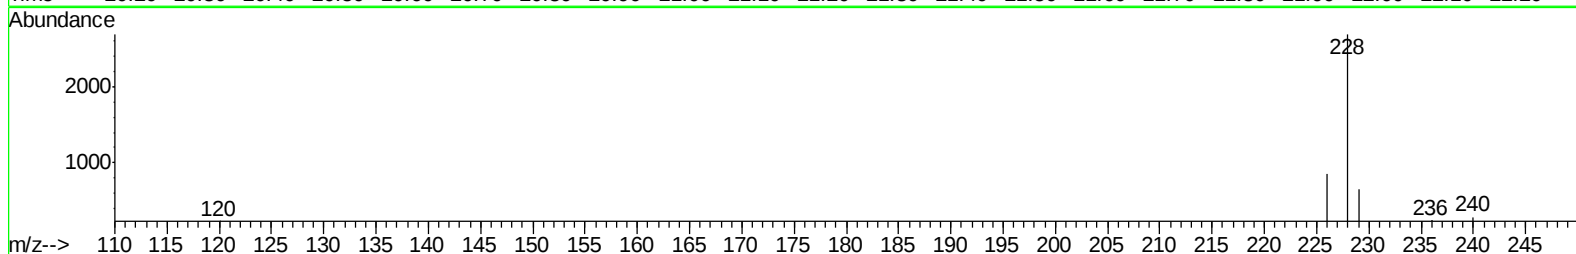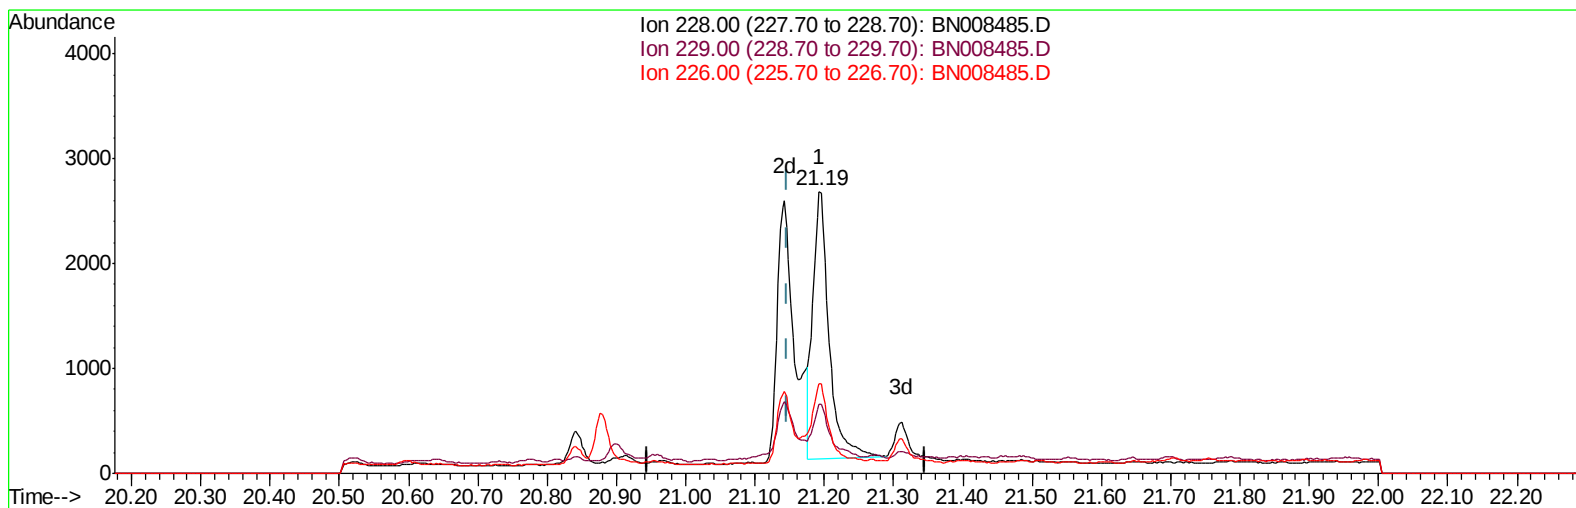

TIC: BN008485.D

(18) Benzo(a)anthracene

21.192min (+0.046) 0.29ng/ul

response 4209

Ion	Exp%	Act%
228.00	100	100
229.00	20.70	24.48
226.00	28.50	31.86
0.00	0.00	0.00