
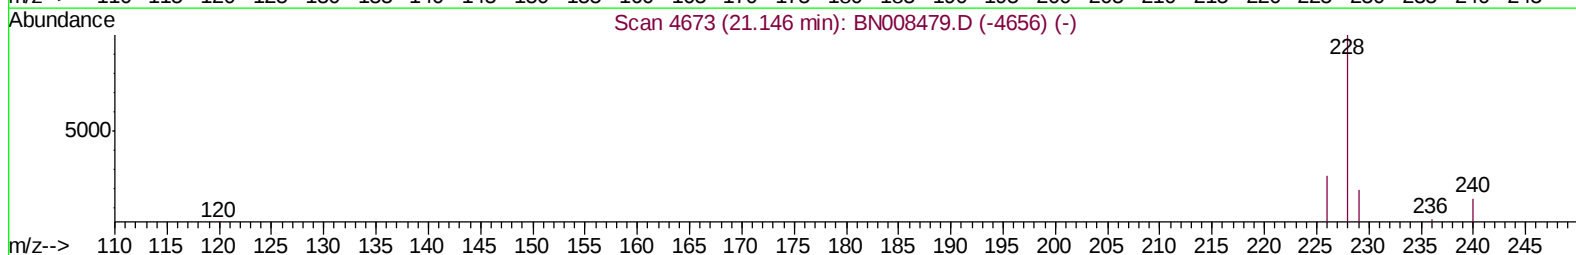
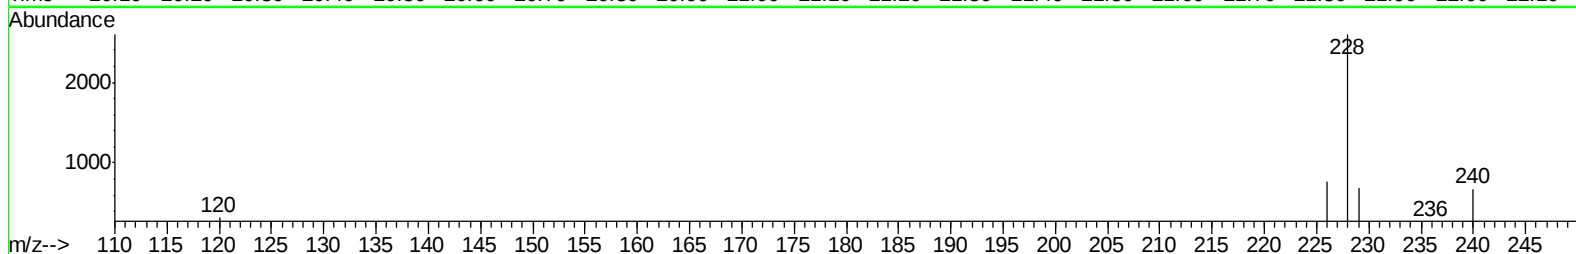


Data File : BN008485.D
Acq On : 07 Nov 2019 15:14
Operator : JU
Sample : K5565-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Nov 08 05:45:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration

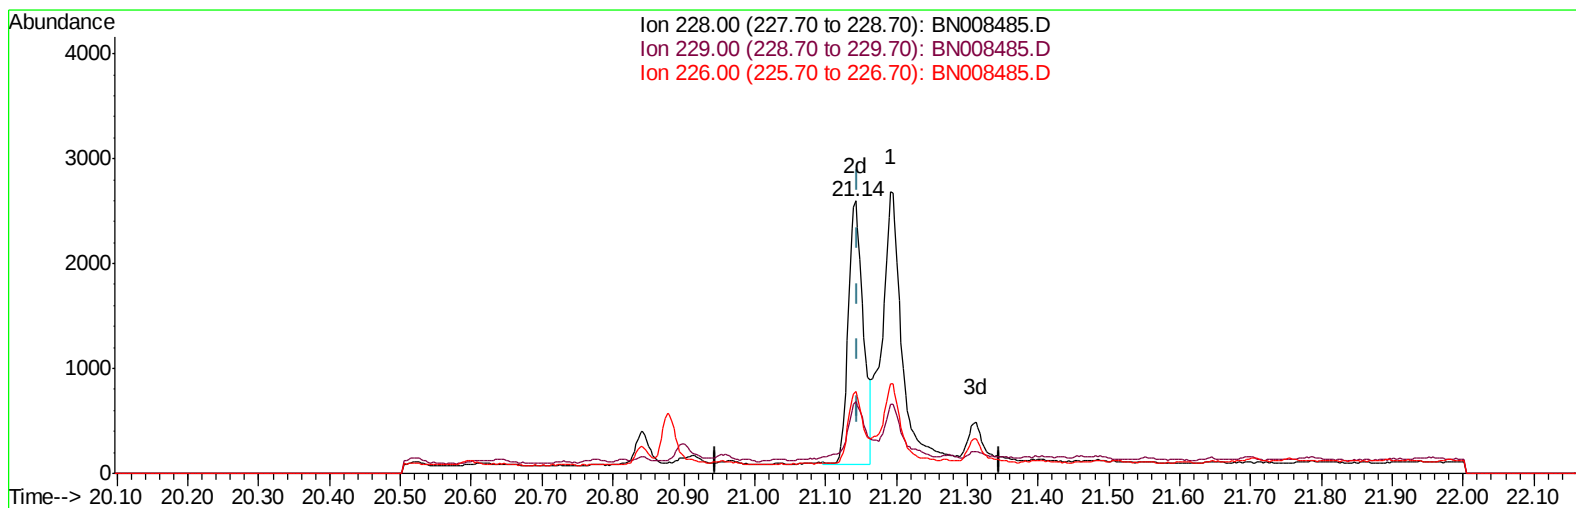

TIC: BN008485.D

(18) Benzo(a)anthracene
21.143min (-0.003) 0.25ng/ul m
response 3699

Ion	Exp%	Act%
228.00	100	100
229.00	20.70	26.37#
226.00	28.50	29.87
0.00	0.00	0.00