
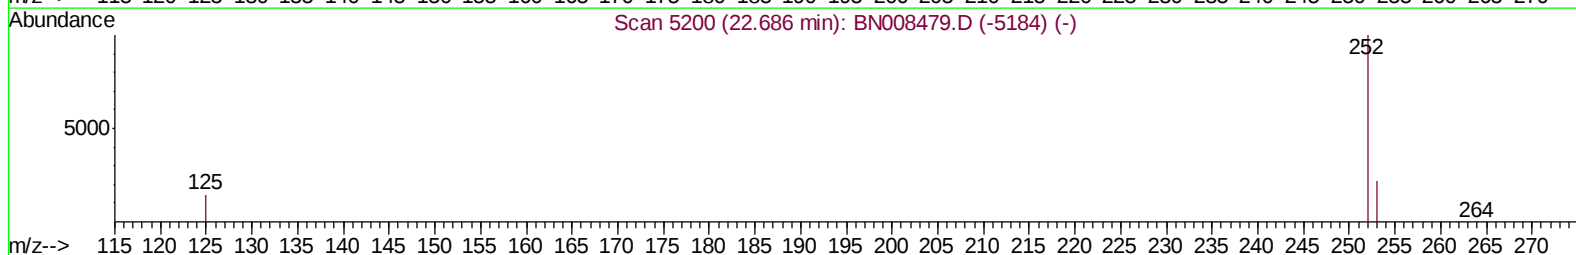
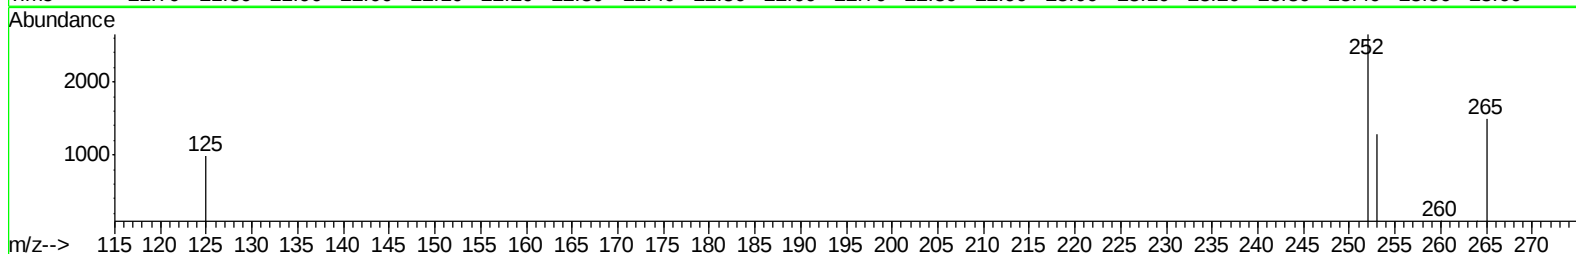


Data File : BN008485.D
Acq On : 07 Nov 2019 15:14
Operator : JU
Sample : K5565-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Nov 08 06:11:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration

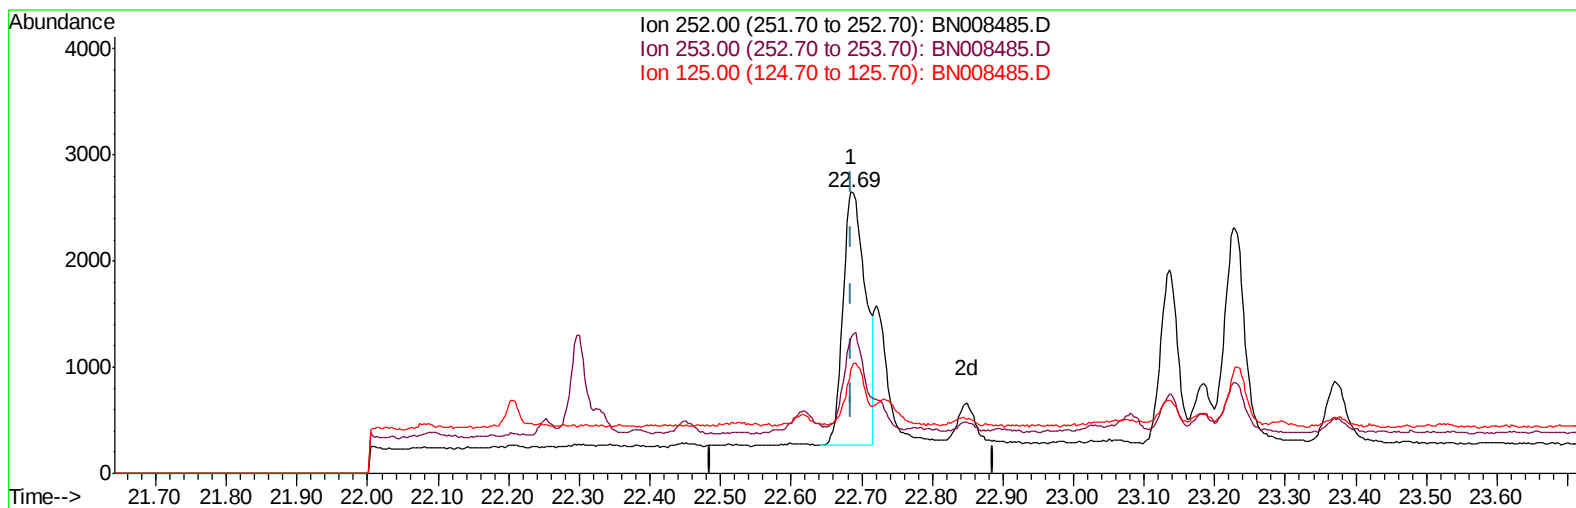

TIC: BN008485.D

(21) Benzo(b)fluoranthene

22.685min (-0.000) 0.34ng/ul m

response 5215

Ion	Exp%	Act%
252.00	100	100
253.00	29.20	48.34
125.00	29.30	36.84
0.00	0.00	0.00