

Data File : BN008485.D

Acq On : 07 Nov 2019 15:14

Operator : JU

Sample : K5565-01

Misc :

ALS Vial : 8 Sample Multiplier: 1




Quant Time: Nov 08 06:11:08 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Nov 08 05:42:36 2019

Response via : Initial Calibration

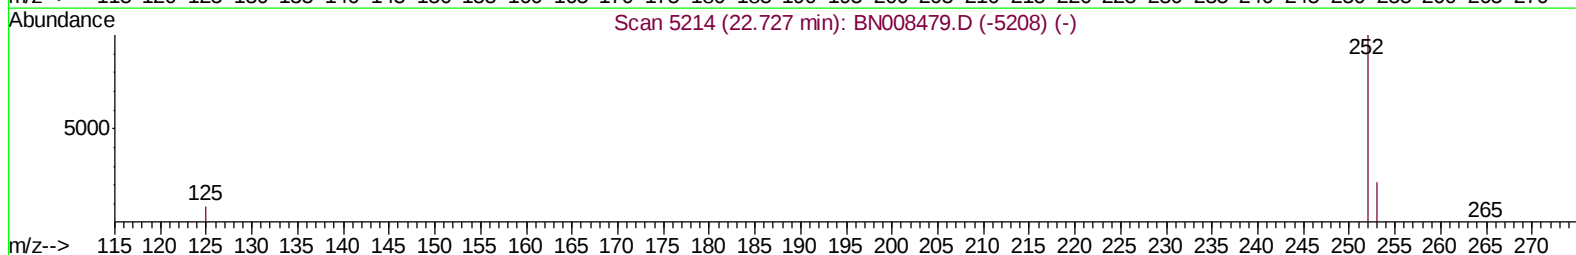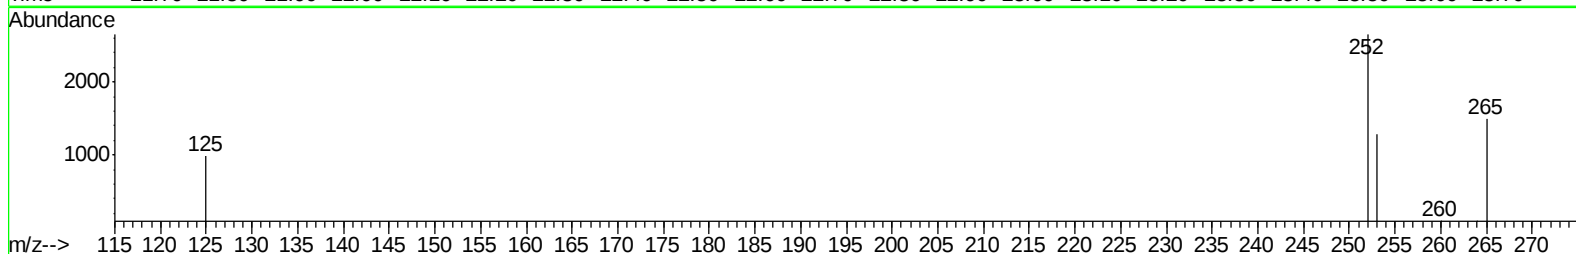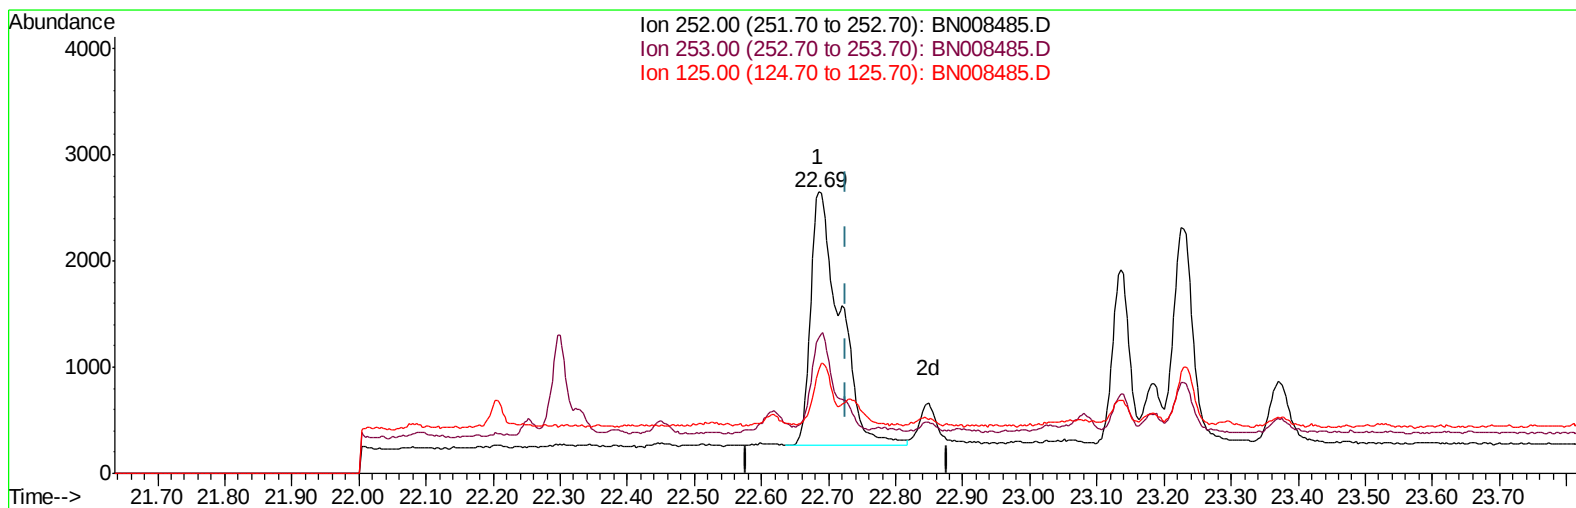

TIC: BN008485.D

(22) Benzo(k)fluoranthene

22.685min (-0.041) 0.41ng/ul

response 7200

Ion	Exp%	Act%
252.00	100	100
253.00	28.30	48.34#
125.00	18.40	36.84#
0.00	0.00	0.00