

Data File : BN008485.D

Acq On : 07 Nov 2019 15:14

Operator : JU

Sample : K5565-01

Misc :

ALS Vial : 8 Sample Multiplier: 1




Quant Time: Nov 08 06:11:08 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Nov 08 05:42:36 2019

Response via : Initial Calibration

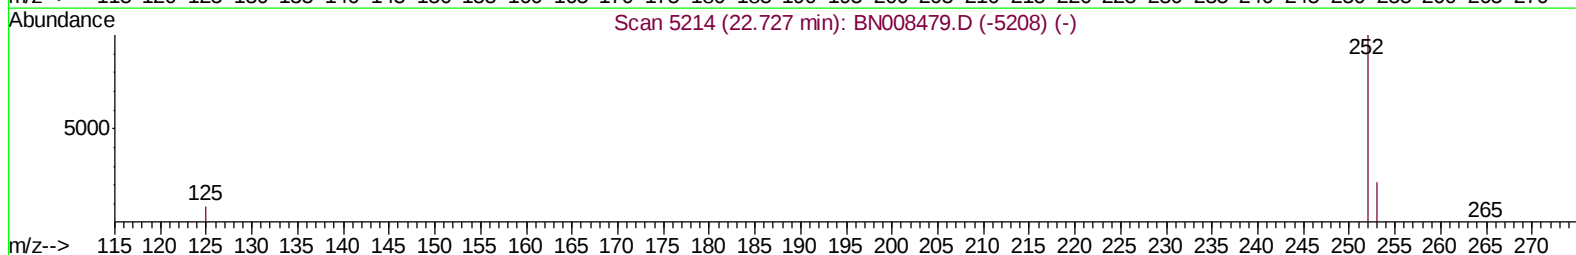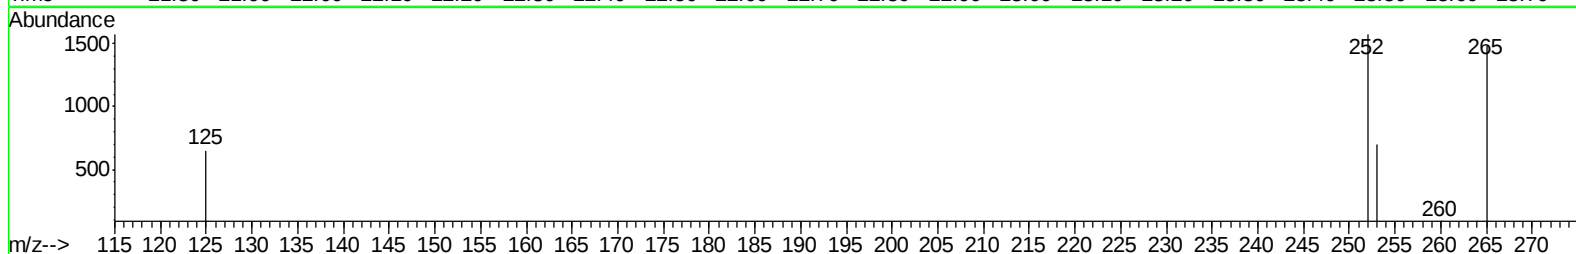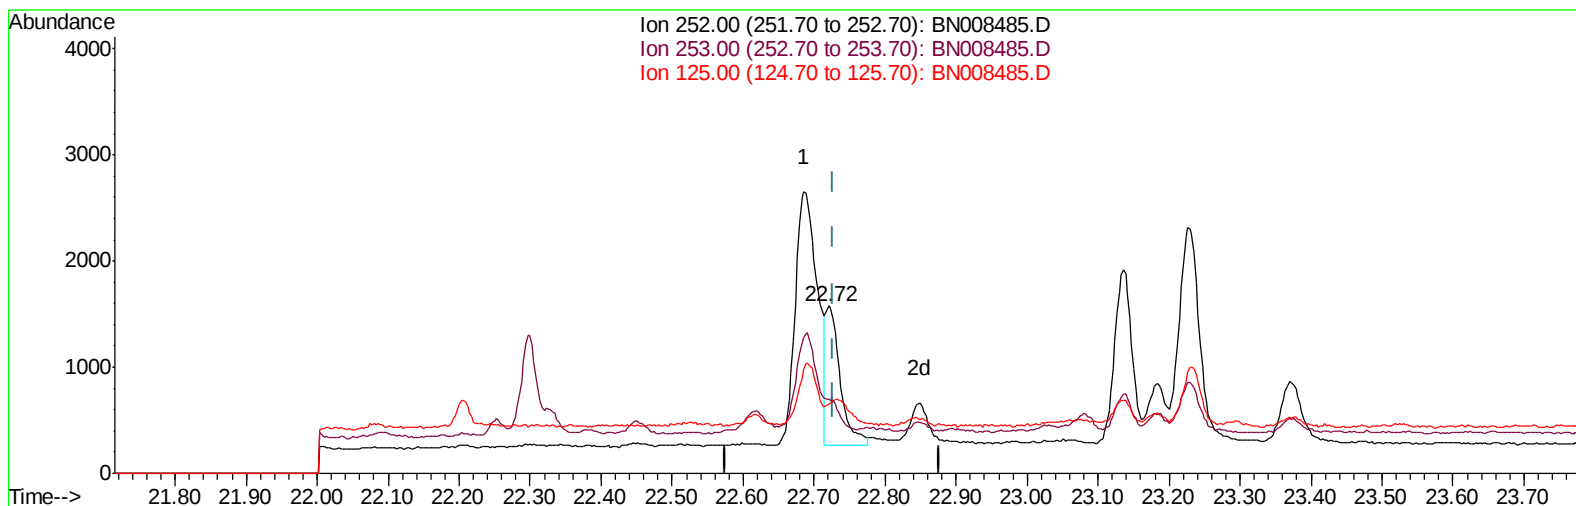

TIC: BN008485.D

(22) Benzo(k)fluoranthene

22.720min (-0.006) 0.11ng/ul m

response 1833

Ion	Exp%	Act%
252.00	100	100
253.00	28.30	44.51#
125.00	18.40	41.21#
0.00	0.00	0.00