
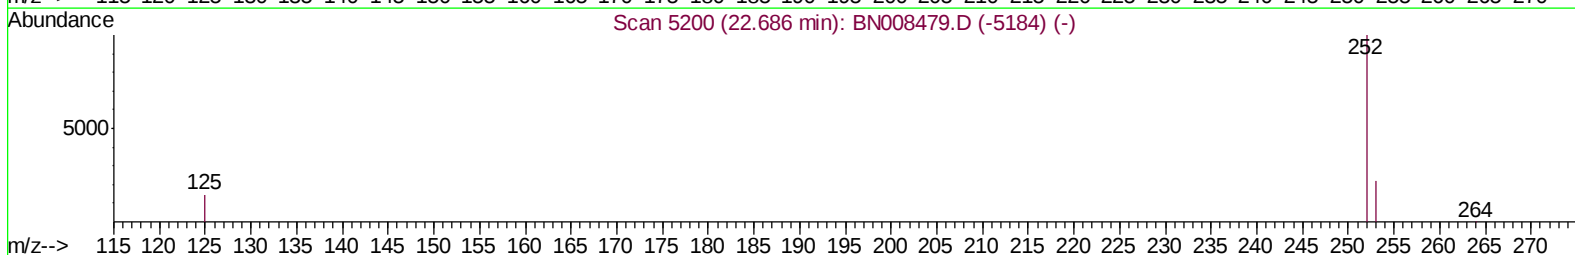
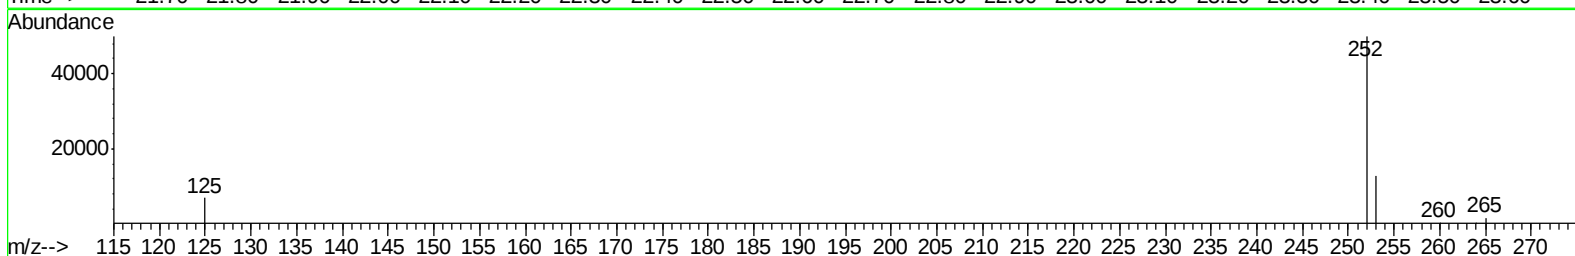


Data File : BN008486.D
Acq On : 07 Nov 2019 15:50
Operator : JU
Sample : K5565-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Nov 08 06:22:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration

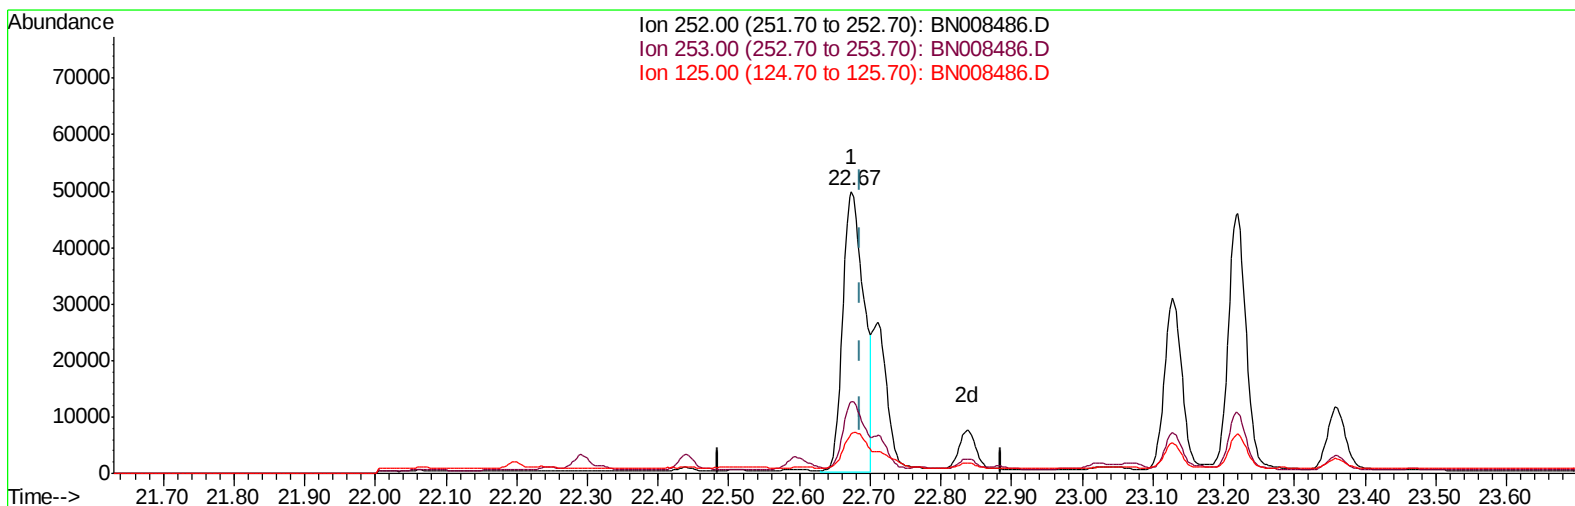

TIC: BN008486.D

(21) Benzo(b)fluoranthene

22.673min (-0.012) 5.56ng/ul m

response 102214

Ion	Exp%	Act%
252.00	100	100
253.00	29.20	25.67
125.00	29.30	13.93
0.00	0.00	0.00