
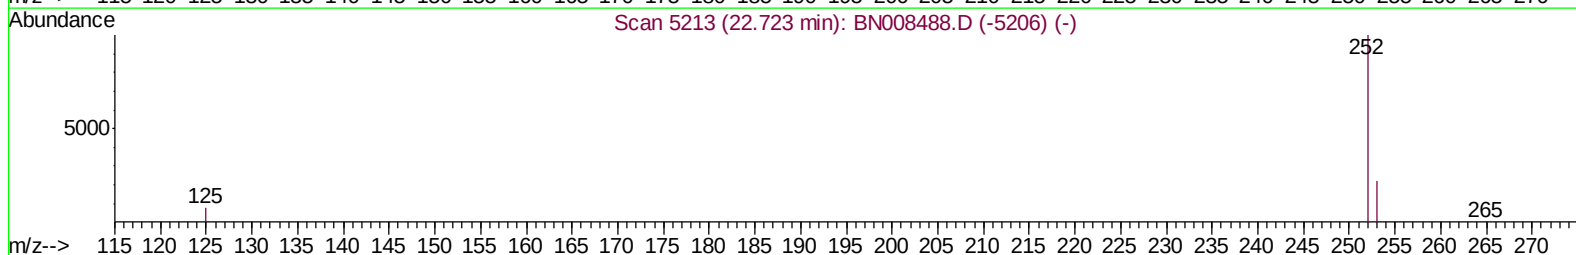
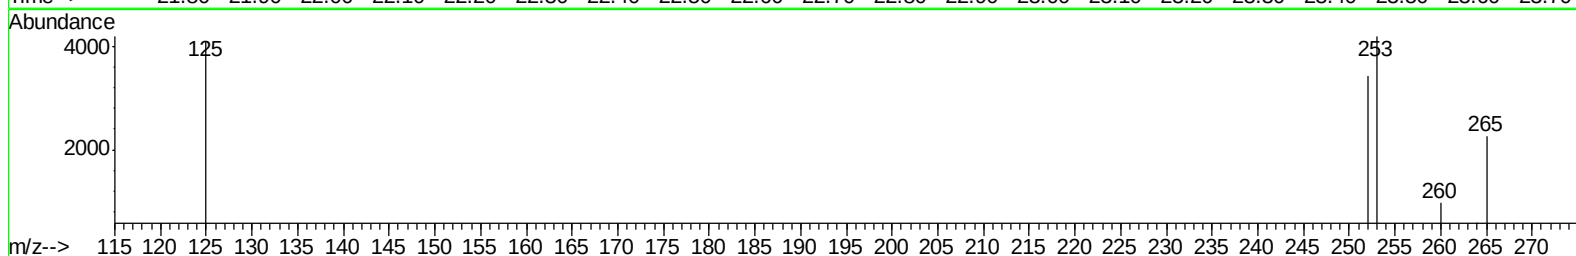


Data File : BN008489.D
Acq On : 07 Nov 2019 17:50
Operator : JU
Sample : K5565-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Nov 08 07:19:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 06:44:20 2019
Response via : Initial Calibration

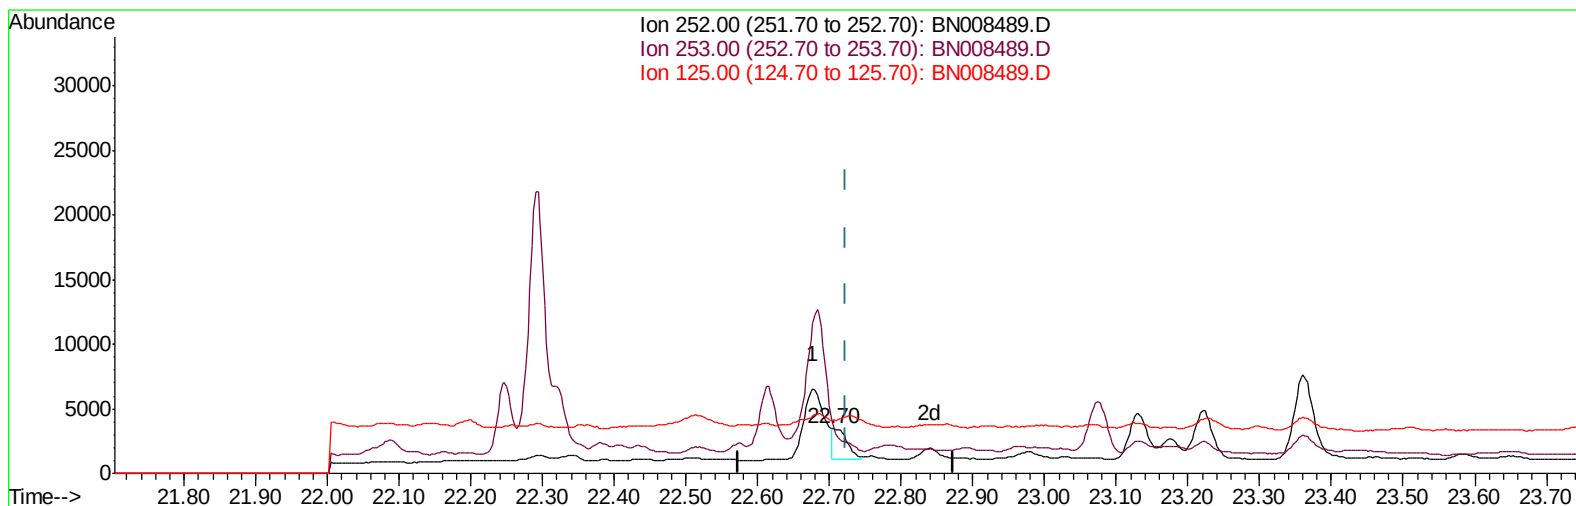

TIC: BN008489.D

(22) Benzo(k)fluoranthene

22.703min (-0.020) 0.10ng/ul m

response 3303

Ion	Exp%	Act%
252.00	100	100
253.00	28.30	122.08#
125.00	18.40	119.43#
0.00	0.00	0.00