
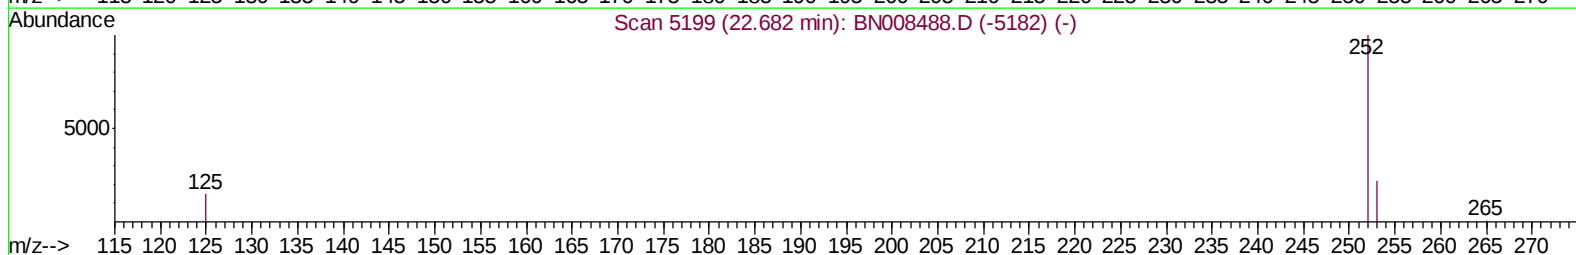
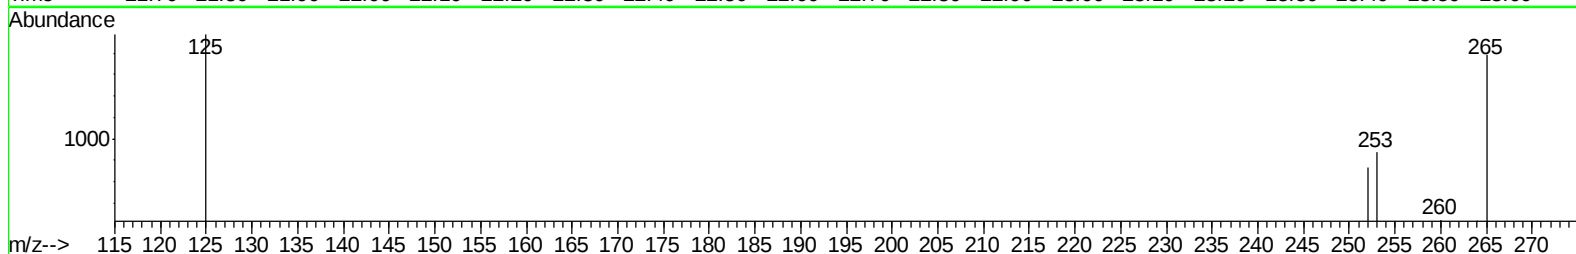


Data File : BN008490.D
Acq On : 07 Nov 2019 18:26
Operator : JU
Sample : K5565-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Nov 08 07:22:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 06:44:20 2019
Response via : Initial Calibration

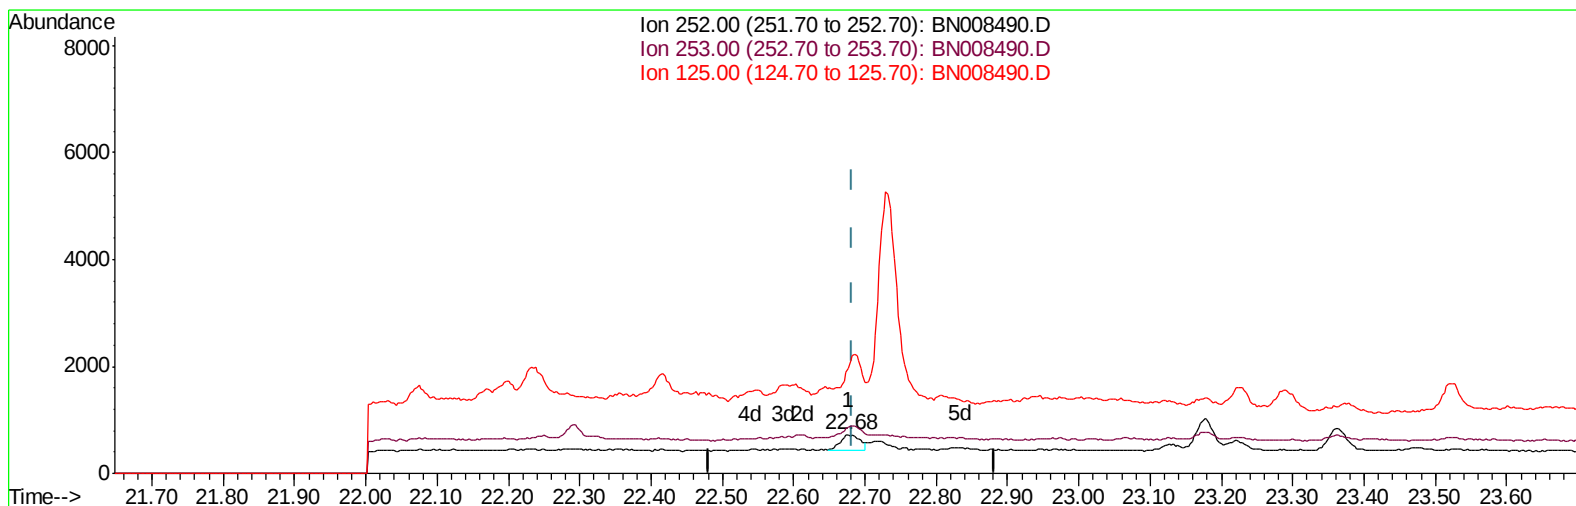

TIC: BN008490.D

(21) Benzo(b)fluoranthene

22.677min (-0.006) 0.03ng/ul m

response 553

Ion	Exp%	Act%
252.00	100	100
253.00	29.20	119.78#
125.00	29.30	271.43#
0.00	0.00	0.00