
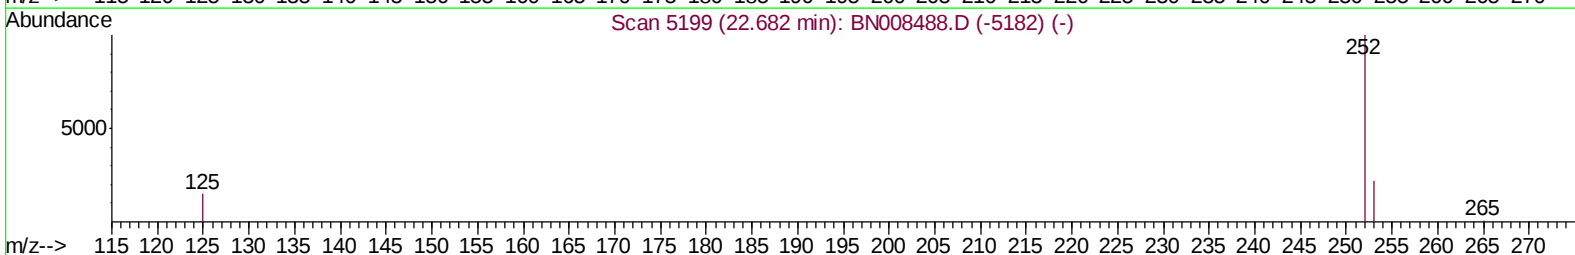
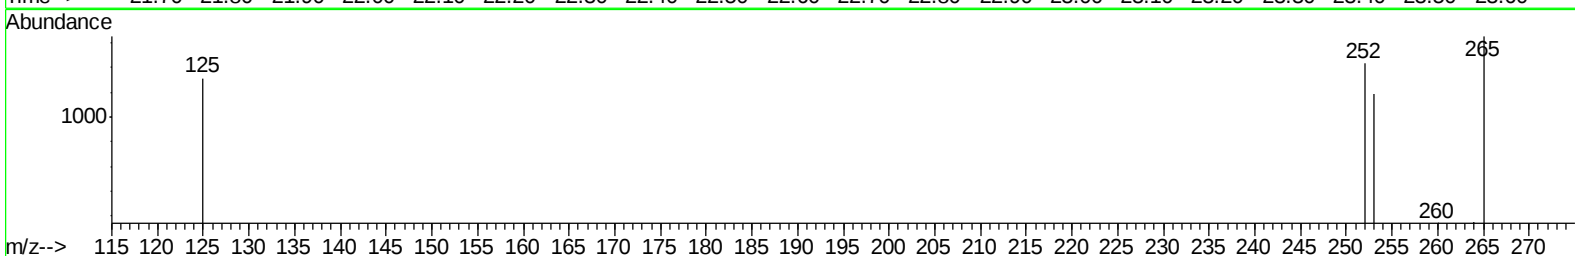


Data File : BN008492.D
Acq On : 07 Nov 2019 19:38
Operator : JU
Sample : K5565-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Nov 08 07:26:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 06:44:20 2019
Response via : Initial Calibration

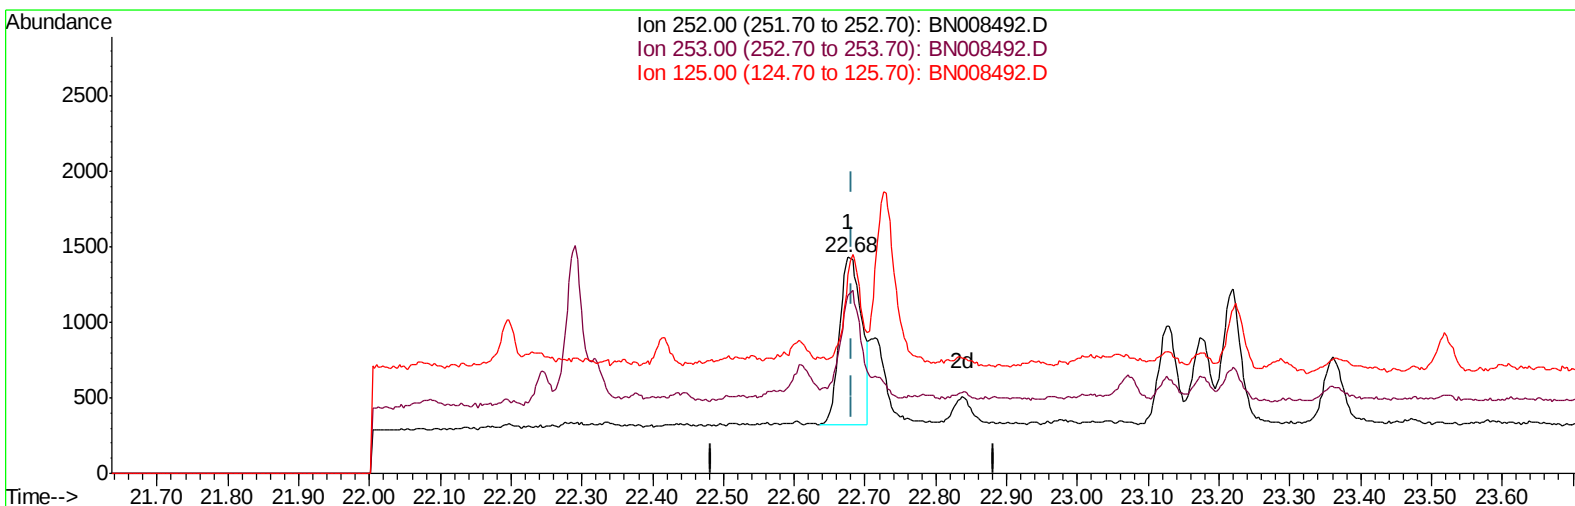

TIC: BN008492.D

(21) Benzo(b)fluoranthene

22.676min (-0.006) 0.15ng/ul m

response 2388

Ion	Exp%	Act%
252.00	100	100
253.00	29.20	82.36#
125.00	29.30	91.70#
0.00	0.00	0.00