
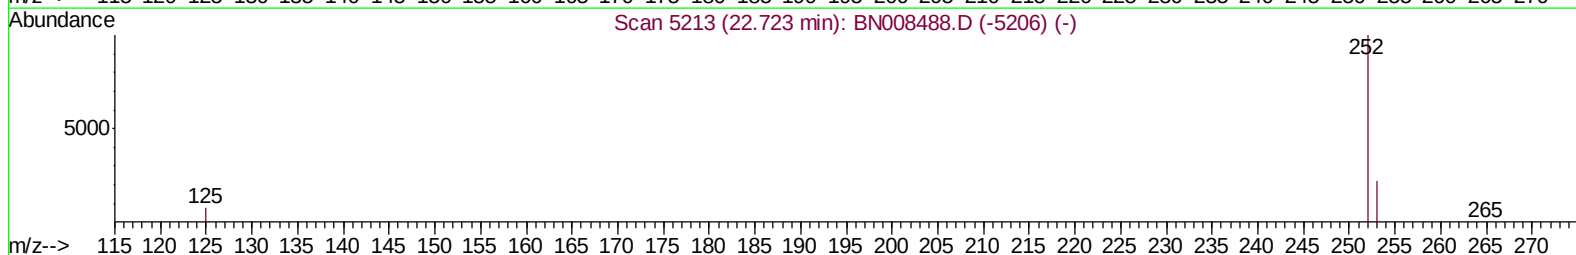
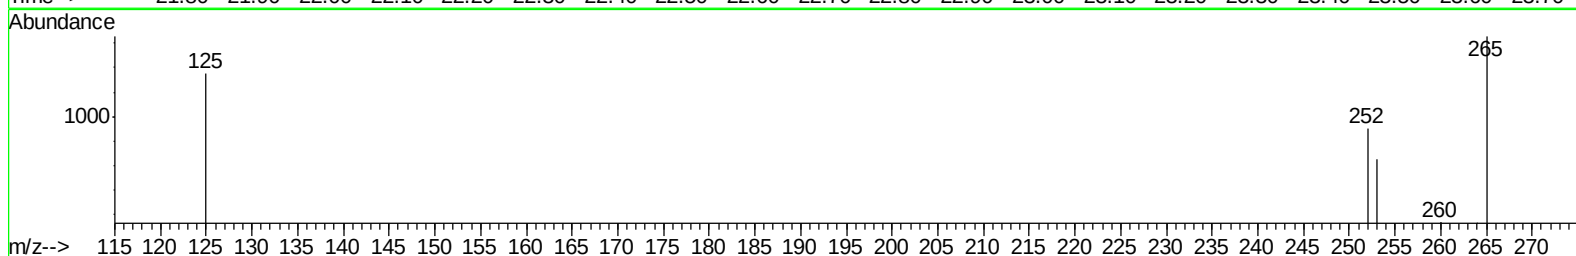


Data File : BN008492.D
Acq On : 07 Nov 2019 19:38
Operator : JU
Sample : K5565-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Nov 08 07:26:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 06:44:20 2019
Response via : Initial Calibration

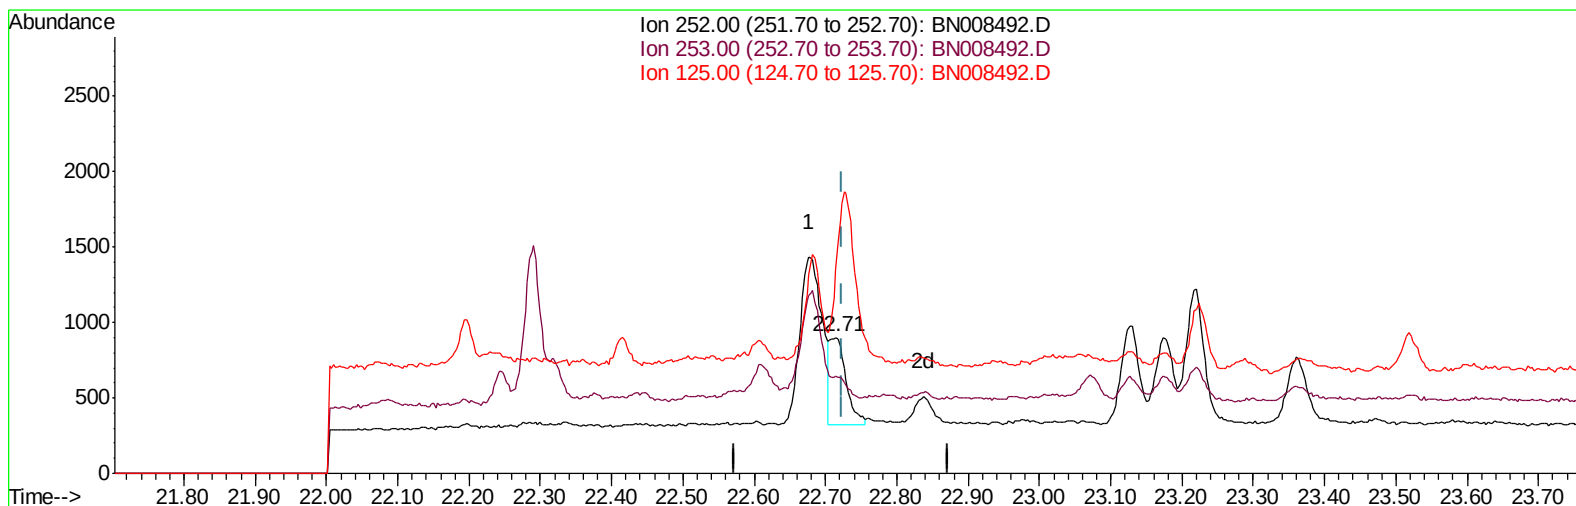

TIC: BN008492.D

(22) Benzo(k)fluoranthene

22.714min (-0.009) 0.05ng/ul m

response 940

Ion	Exp%	Act%
252.00	100	100
253.00	28.30	71.89#
125.00	18.40	149.89#
0.00	0.00	0.00