

Data File : BN008484.D
Acq On : 07 Nov 2019 14:38
Operator : JU
Sample : PB124433BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK33

Quant Time: Nov 08 05:45:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	1291	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.31	136	5148	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.19	164	2633	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.95
16) Chrysene-d12	21.17	240	3737	0.40	ng/ul	0.00
20) Perylene-d12	23.33	264	6030	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.93	152	2745	0.34	ng/ul	0.00
14) Fluoranthene-d10	18.99	212	5762	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.35	202	861	0.047	ng/ul#	1
23) Benzo(a)pyrene	23.19	252	1940	0.086	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN008484.D
Acq On : 07 Nov 2019 14:38
Operator : JU
Sample : PB124433BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK33

Quant Time: Nov 08 05:45:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration




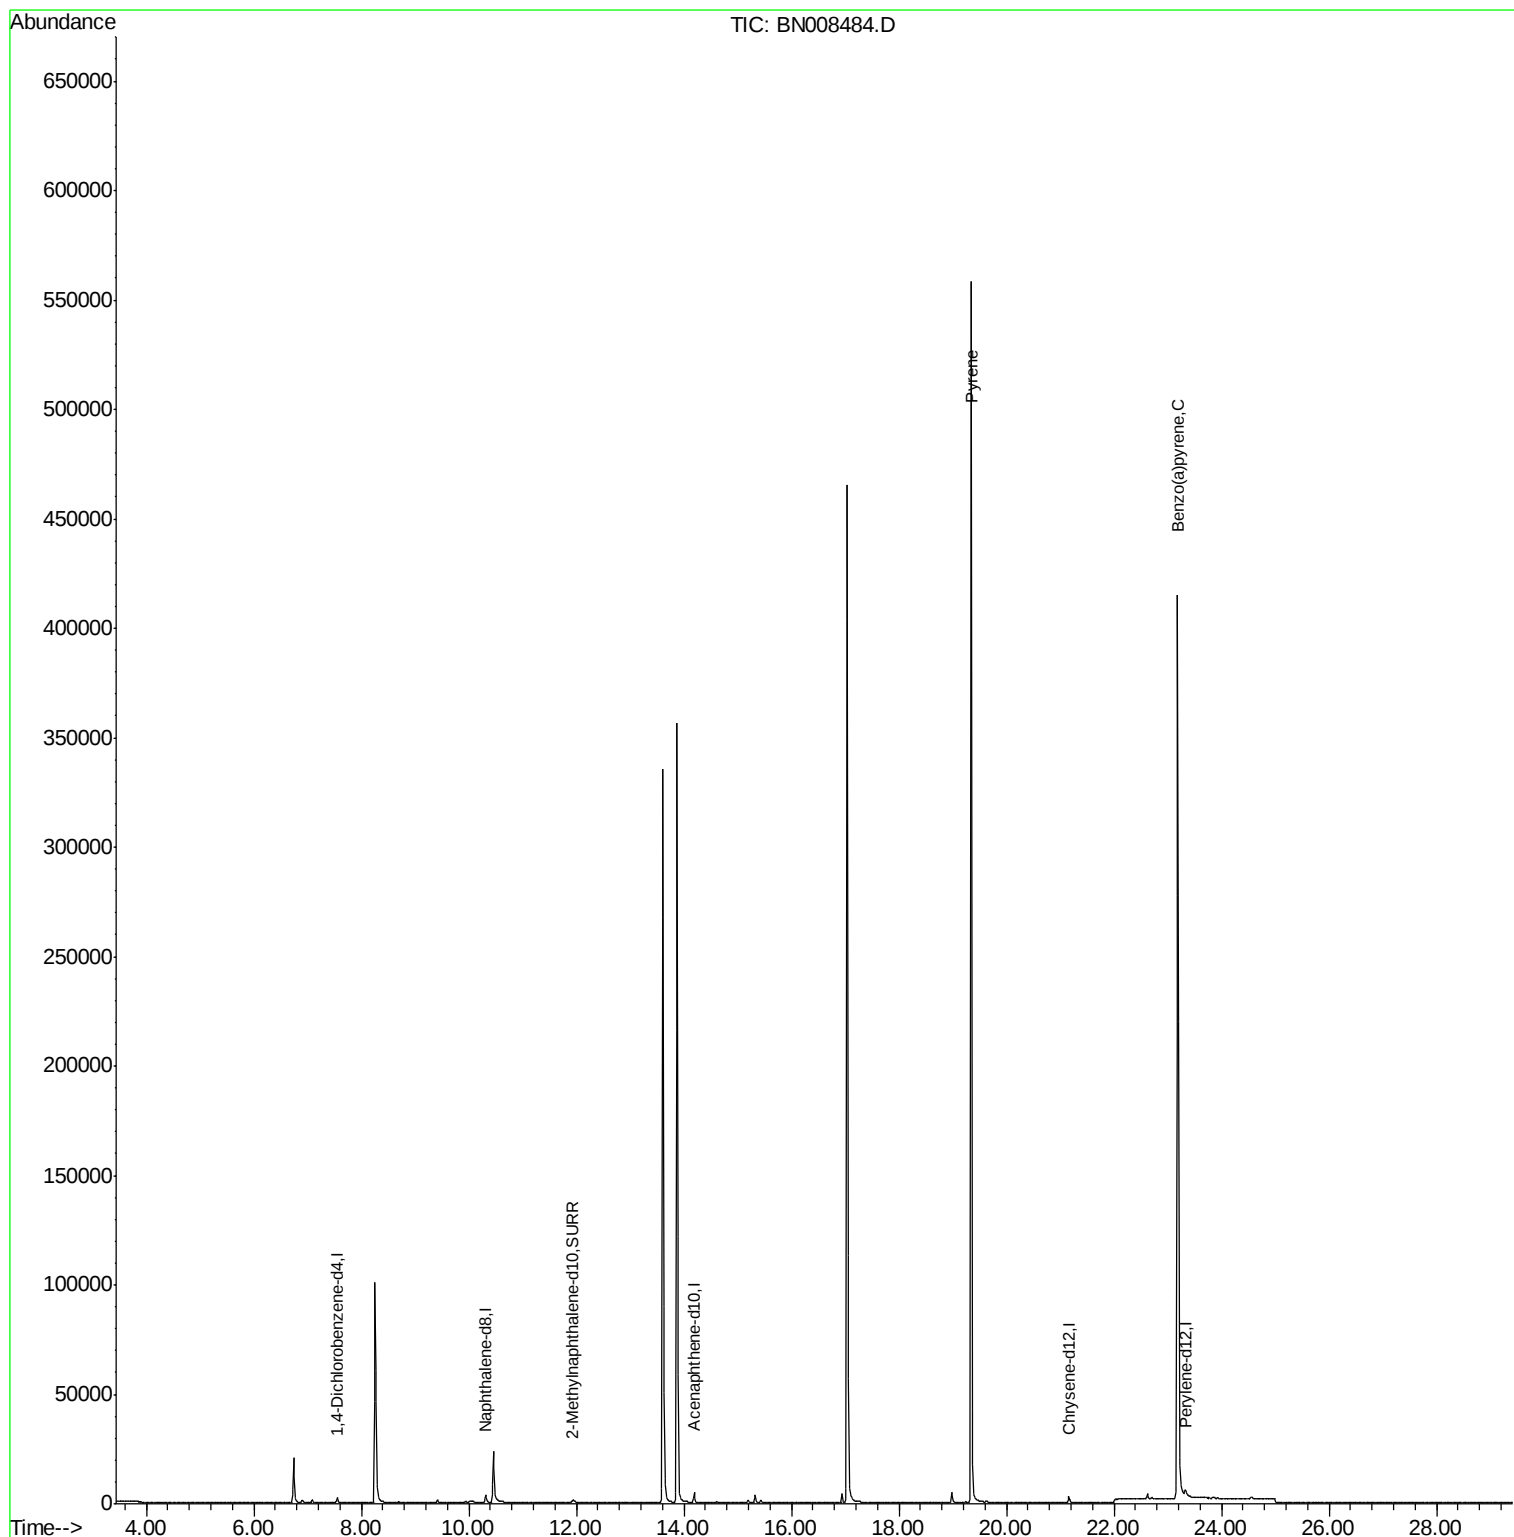


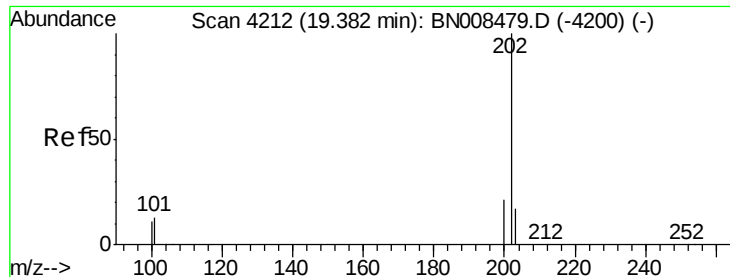

#17
 Pyrene
 Concen: 0.047 ng/ul
 RT: 19.35 min Scan# 4205
 Delta R.T. -0.03 min
 Lab File: BN008484.D
 Acq: 07 Nov 2019 14:38

Instrument :
 BNA_N
 ClientSampleId :
 SBLK33

Tgt Ion:202 Resp: 861
 Ion Ratio Lower Upper
 202 100
 101 183.3 11.6 17.4#
 100 1220.6 9.4 14.0#

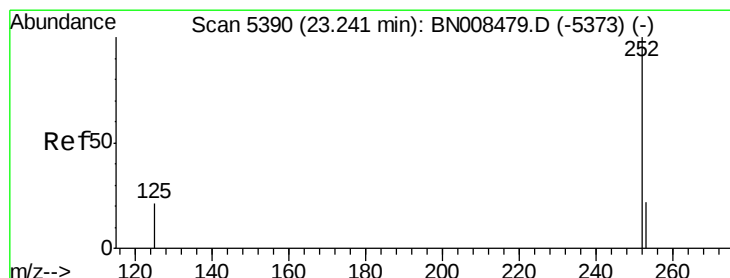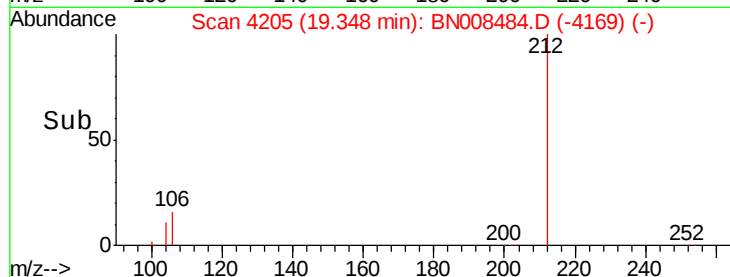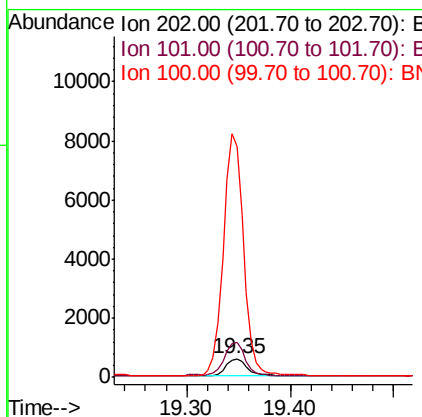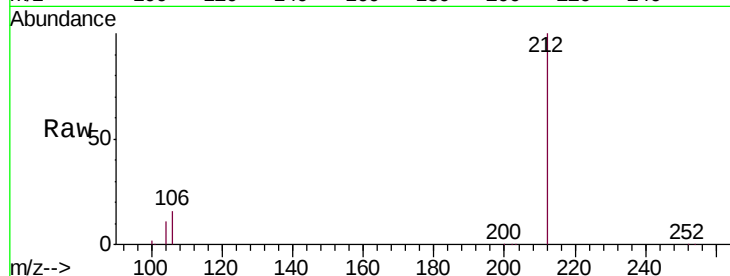

#23
 Benzo(a)pyrene
 Concen: 0.086 ng/ul
 RT: 23.19 min Scan# 5372
 Delta R.T. -0.05 min
 Lab File: BN008484.D
 Acq: 07 Nov 2019 14:38

Tgt Ion:252 Resp: 1940
 Ion Ratio Lower Upper
 252 100
 253 45.8 27.2 40.8#
 125 43.9 37.0 55.6

