

Data File : BN008487.D
Acq On : 07 Nov 2019 16:25
Operator : JU
Sample : K5565-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLNA2

Quant Time: Nov 08 05:45:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	1524	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.31	136	6547	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.19	164	3761	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.95
16) Chrysene-d12	21.16	240	5223	0.40	ng/ul	0.00
20) Perylene-d12	23.32	264	6550	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.92	152	2710	0.26	ng/ul	0.00
14) Fluoranthene-d10	18.98	212	6022	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.34	202	872	0.034	ng/ul#	1
23) Benzo(a)pyrene	23.18	252	1460	0.059	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN008487.D
Acq On : 07 Nov 2019 16:25
Operator : JU
Sample : K5565-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLNA2

Quant Time: Nov 08 05:45:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration




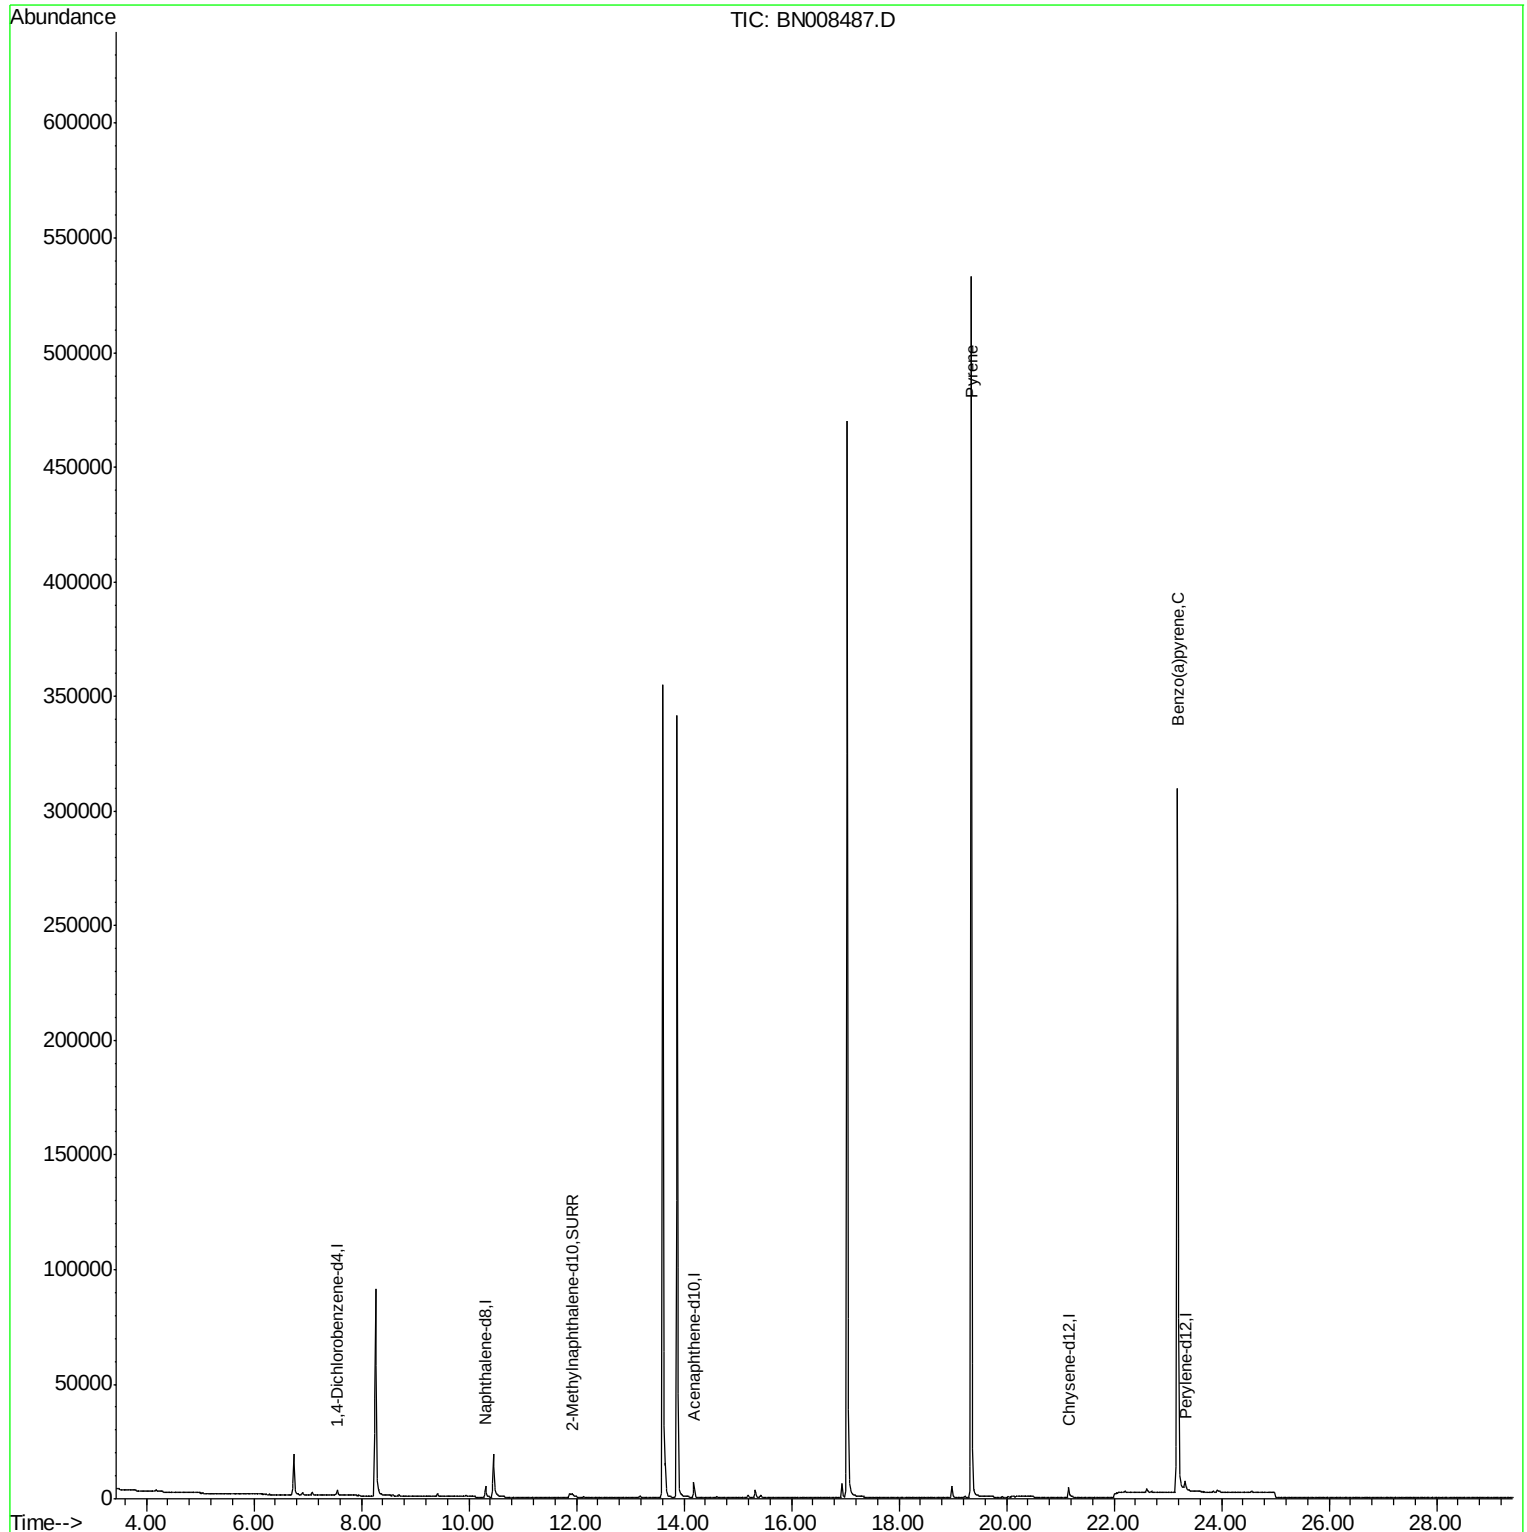


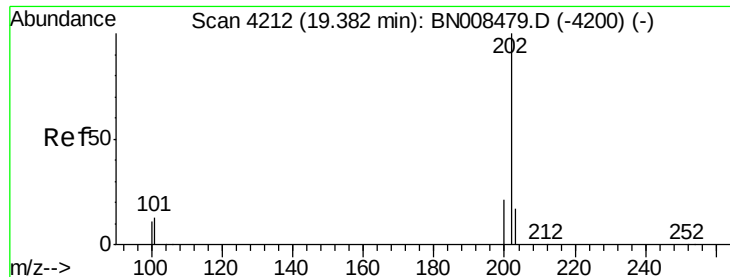

#17
 Pyrene
 Concen: 0.034 ng/ul
 RT: 19.34 min Scan# 4204
 Delta R.T. -0.04 min
 Lab File: BN008487.D
 Acq: 07 Nov 2019 16:25

Instrument :
 BNA_N
 ClientSampleId :
 JLNA2

Tgt Ion:202 Resp: 872
 Ion Ratio Lower Upper
 202 100
 101 179.3 11.6 17.4#
 100 1189.1 9.4 14.0#

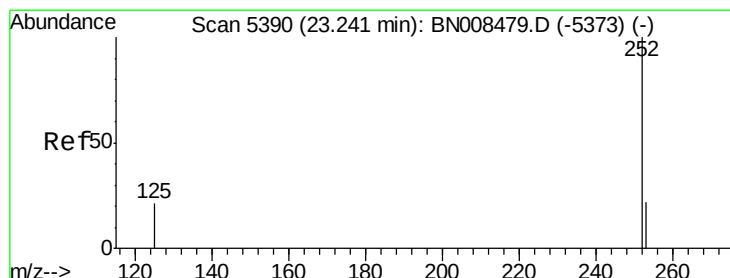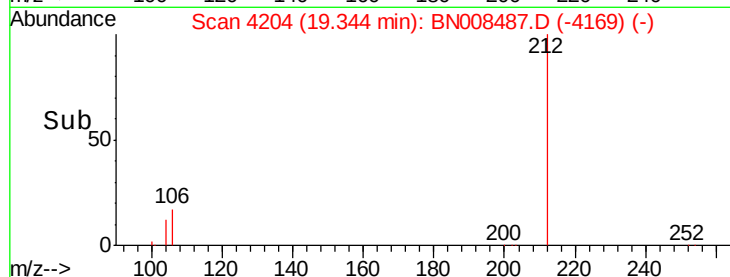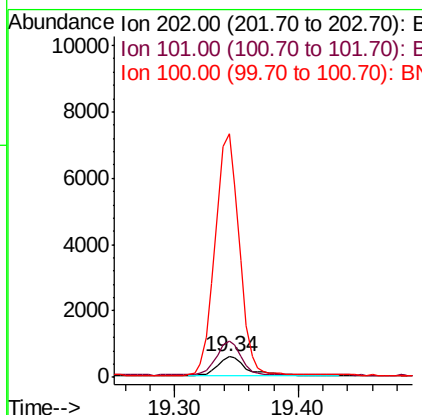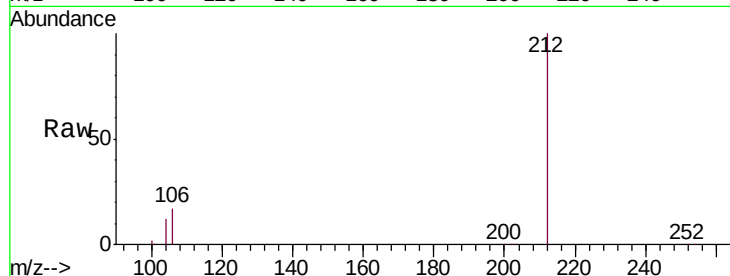

#23
 Benzo(a)pyrene
 Concen: 0.059 ng/ul
 RT: 23.18 min Scan# 5369
 Delta R.T. -0.06 min
 Lab File: BN008487.D
 Acq: 07 Nov 2019 16:25

Tgt Ion:252 Resp: 1460
 Ion Ratio Lower Upper
 252 100
 253 54.8 27.2 40.8#
 125 60.2 37.0 55.6#

