

Data File : BN008493.D
Acq On : 07 Nov 2019 20:14
Operator : JU
Sample : K5565-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLNA7

Quant Time: Nov 08 06:47:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 06:44:20 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	1603	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	6818	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	3900	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.94	188	7020	0.40	ng/ul	0.00
16) Chrysene-d12	21.15	240	4838	0.40	ng/ul	0.00
20) Perylene-d12	23.32	264	6354	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.91	152	1850	0.17	ng/ul	0.00
14) Fluoranthene-d10	18.98	212	3752	0.18	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.36	128	686	0.035	ng/ul#	73
5) 2-Methylnaphthalene	11.99	142	392	0.030	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN008493.D
Acq On : 07 Nov 2019 20:14
Operator : JU
Sample : K5565-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLNA7

Quant Time: Nov 08 06:47:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 06:44:20 2019
Response via : Initial Calibration

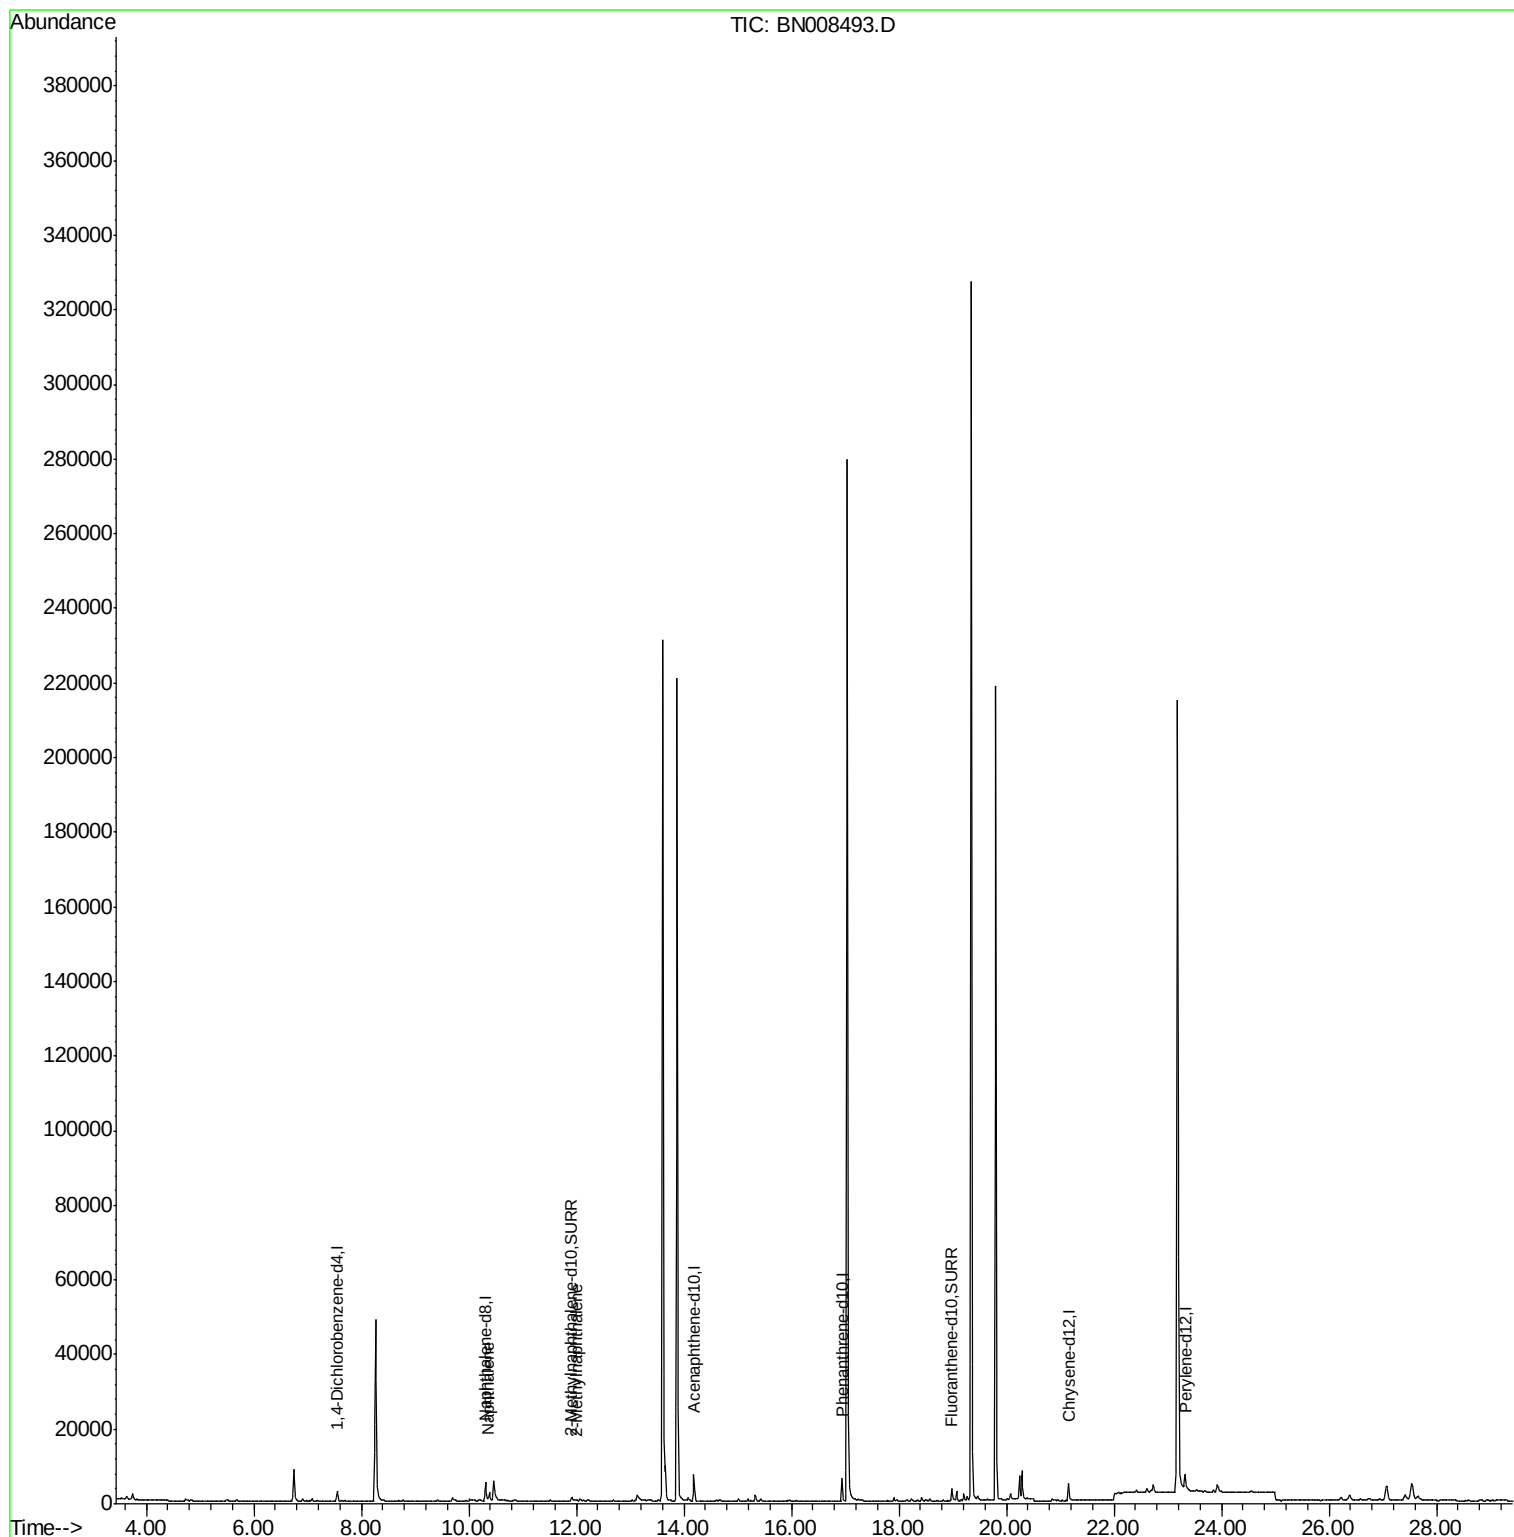

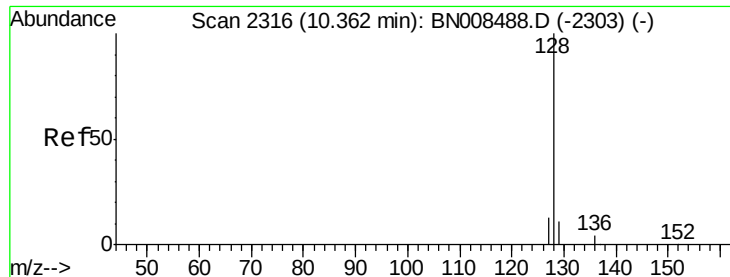

#3

Naphthalene

Concen: 0.035 ng/ul

RT: 10.36 min Scan# 2315

Delta R.T. -0.01 min

Lab File: BN008493.D

Acq: 07 Nov 2019 20:14

Instrument :

BNA_N

ClientSampleId :

JLNA7


Tgt Ion:128 Resp: 686

Ion Ratio Lower Upper

128 100

129 24.9 10.0 15.0#




127 23.6 11.6 17.4#

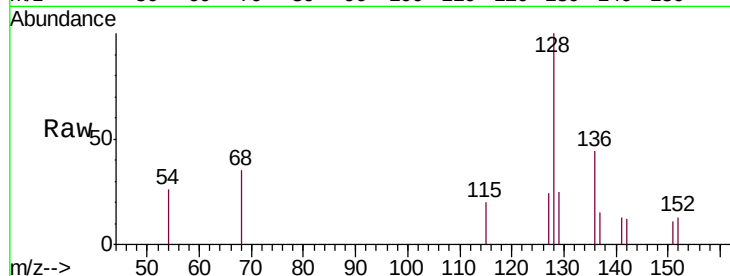

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

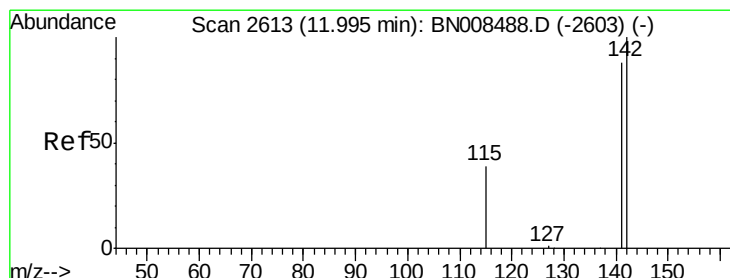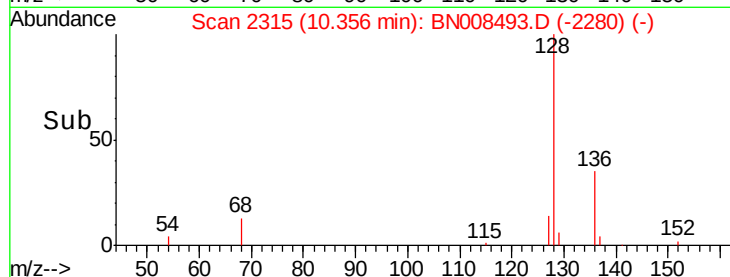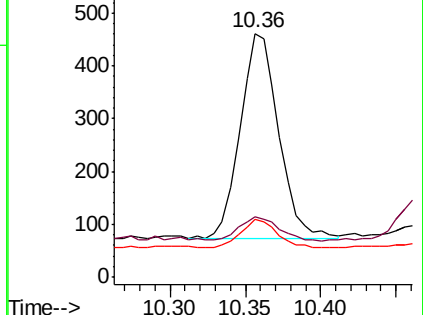

#5

2-Methylnaphthalene

Concen: 0.030 ng/ul

RT: 11.99 min Scan# 2612

Delta R.T. -0.01 min

Lab File: BN008493.D


Acq: 07 Nov 2019 20:14

Tgt Ion:142 Resp: 392

Ion Ratio Lower Upper

142 100

141 94.9 72.8 109.2

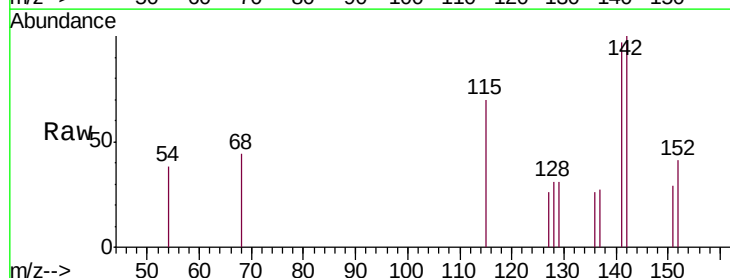

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

