

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (QT Reviewed)


Data File : BN008483.D
Acq On : 07 Nov 2019 14:02
Operator : JU
Sample : PB124530BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK30

Manual Integrations
APPROVED

mohammad
11/11/2019 8:07:55 AM

Quant Time: Nov 08 06:03:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration

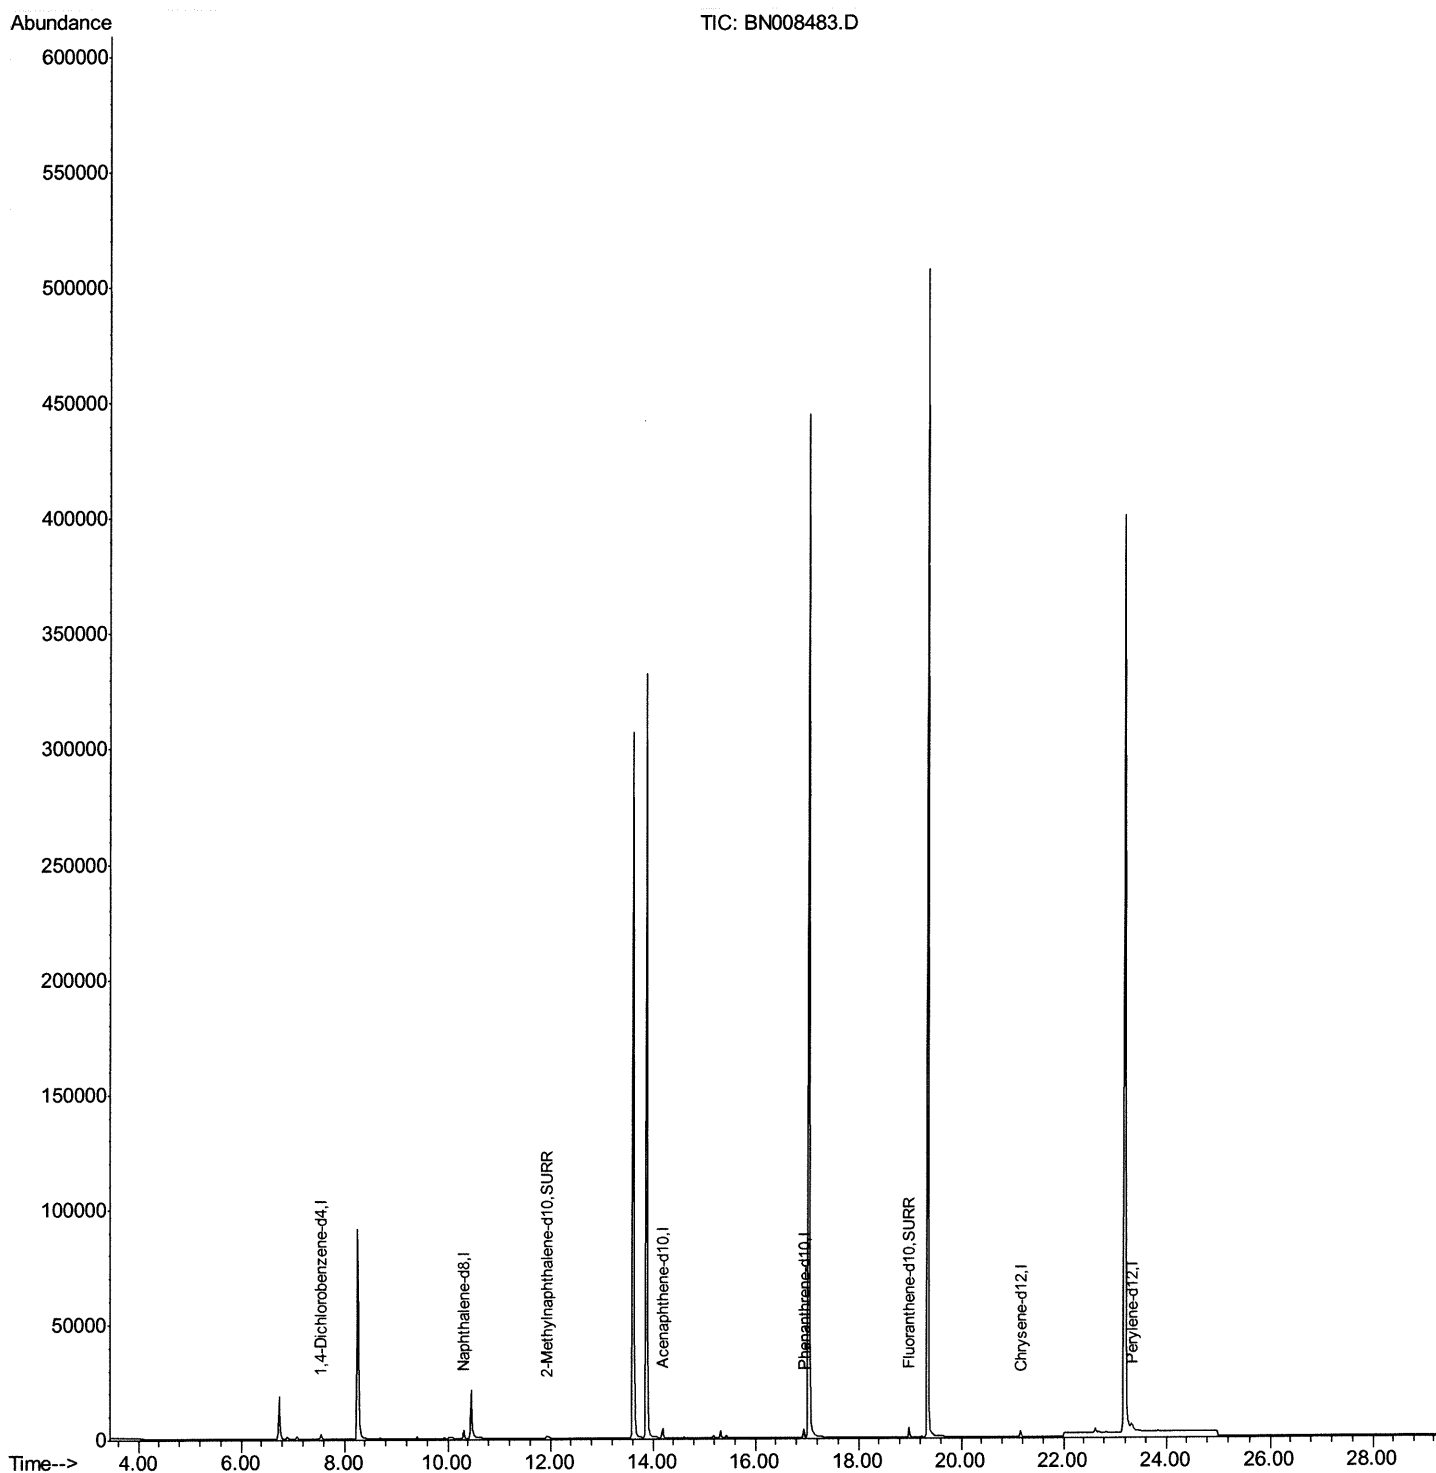

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (Qedit)




Data File : BN008483.D
Acq On : 07 Nov 2019 14:02
Operator : JU
Sample : PB124530BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK30

Manual Integrations
APPROVED

mohammad
11/11/2019 8:07:55 AM

Quant Time: Nov 08 05:45:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration

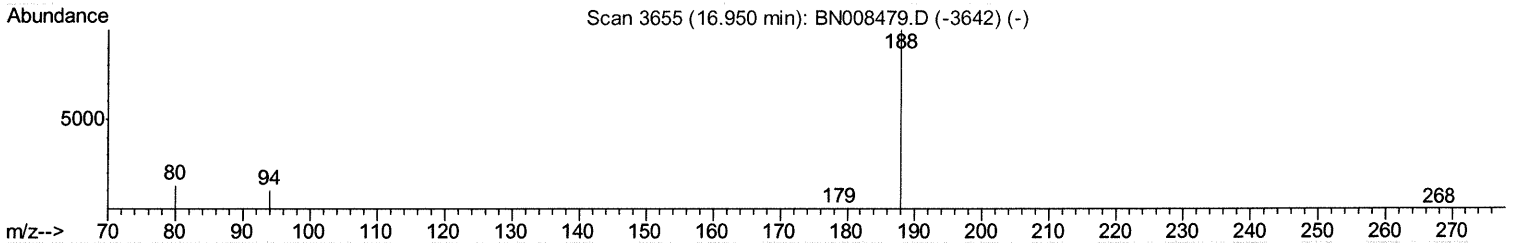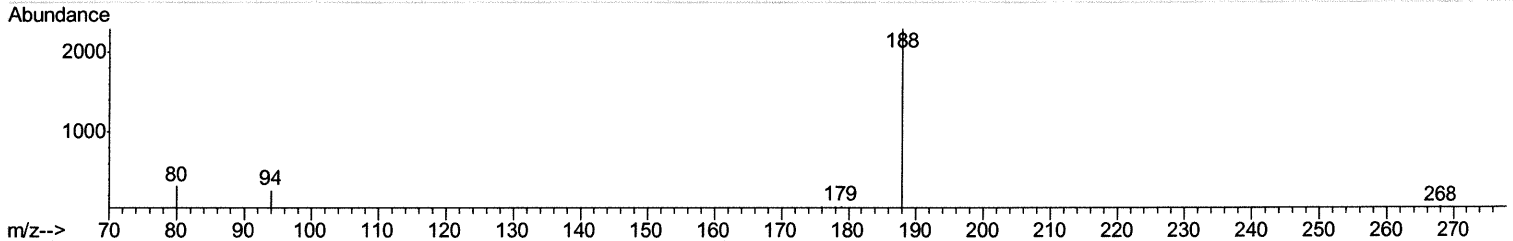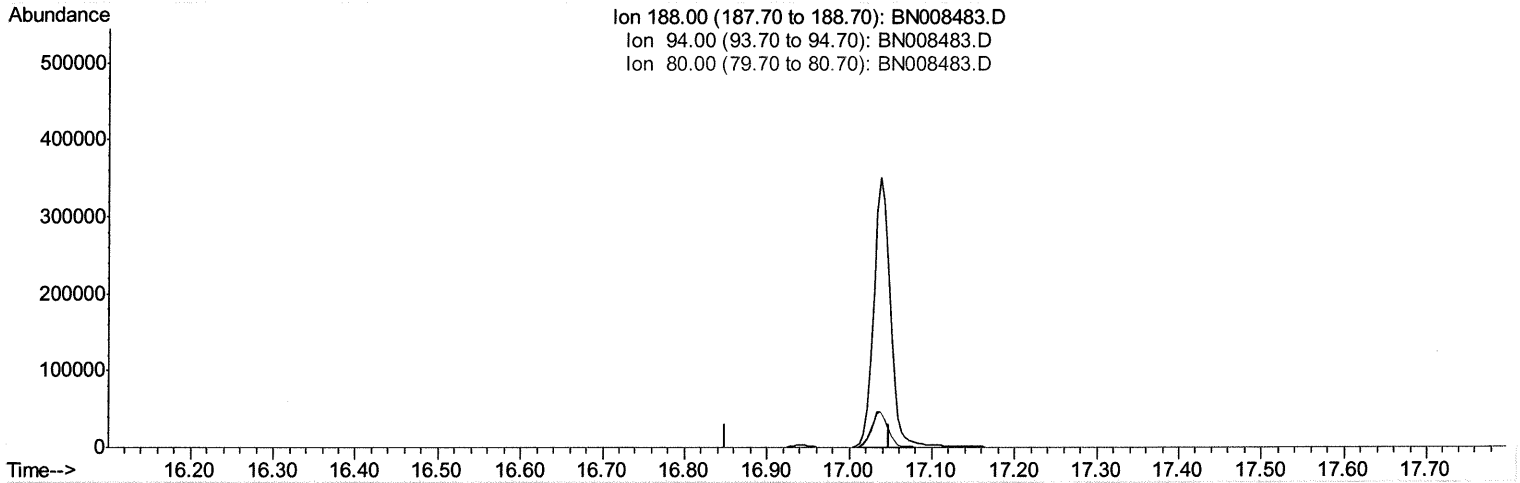

TIC: BN008483.D

(10) Phenanthrene-d10 (I)

16.950min (-16.950) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	12.40	0.00#
80.00	15.50	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (Qedit)




Data File : BN008483.D
Acq On : 07 Nov 2019 14:02
Operator : JU
Sample : PB124530BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK30

Manual Integrations
APPROVED

mohammad
11/11/2019 8:07:55 AM

Quant Time: Nov 08 05:45:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration

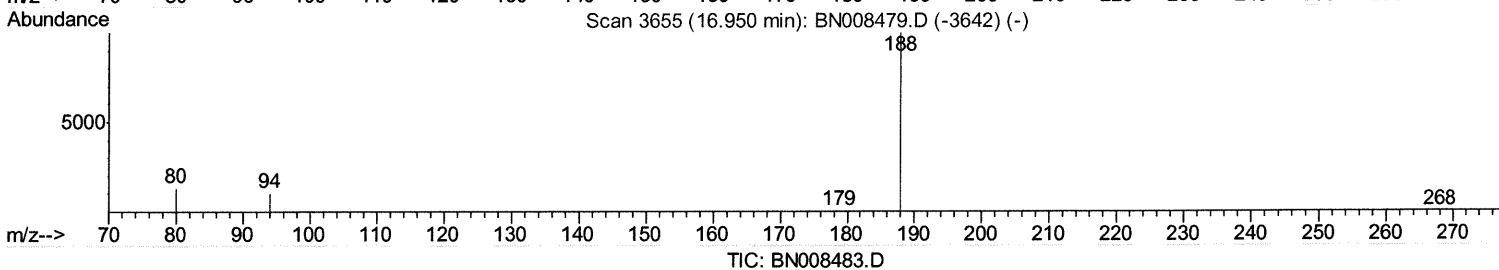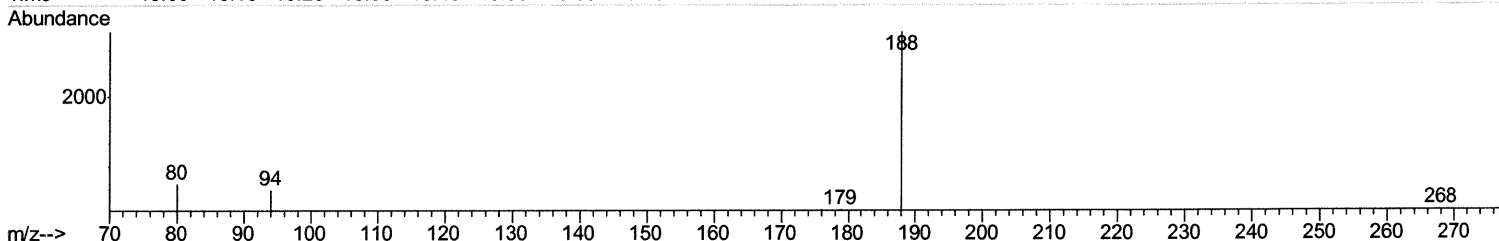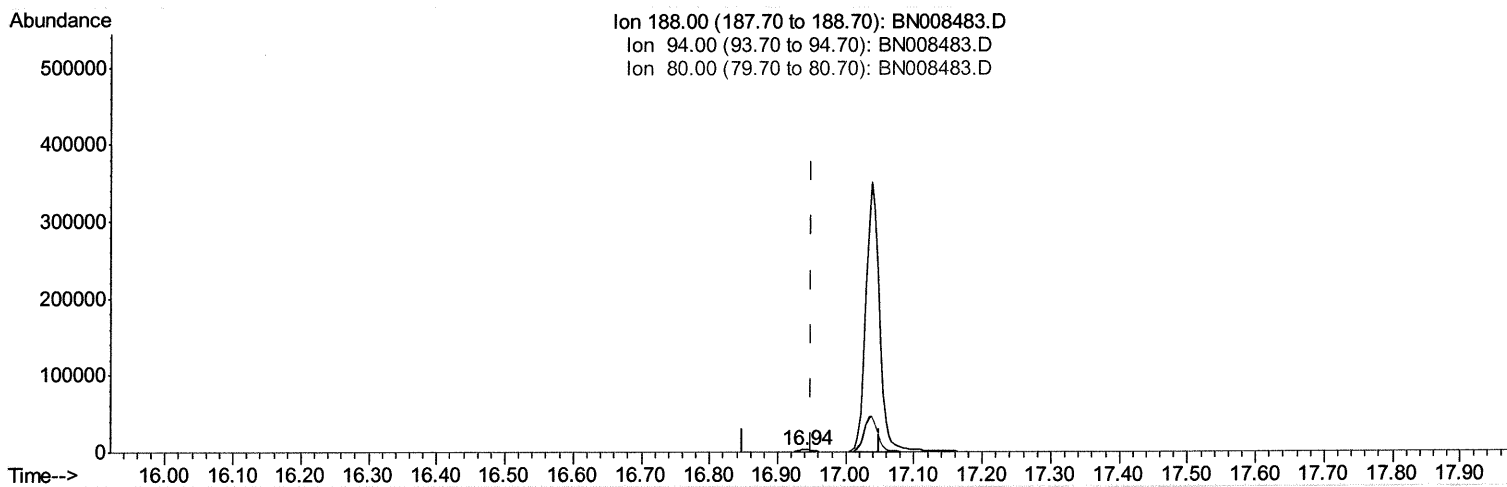

(10) Phenanthrene-d10 (I)

16.941min (-0.009) 0.40ng/ul m

24 11/11/19

response 4518

Ion	Exp%	Act%
188.00	100	100
94.00	12.40	12.83
80.00	15.50	16.01
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (Qedit)




Data File : BN008483.D
Acq On : 07 Nov 2019 14:02
Operator : JU
Sample : PB124530BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK30

Manual Integrations
APPROVED

mohammad
11/11/2019 8:07:55 AM

Quant Time: Nov 08 06:00:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration

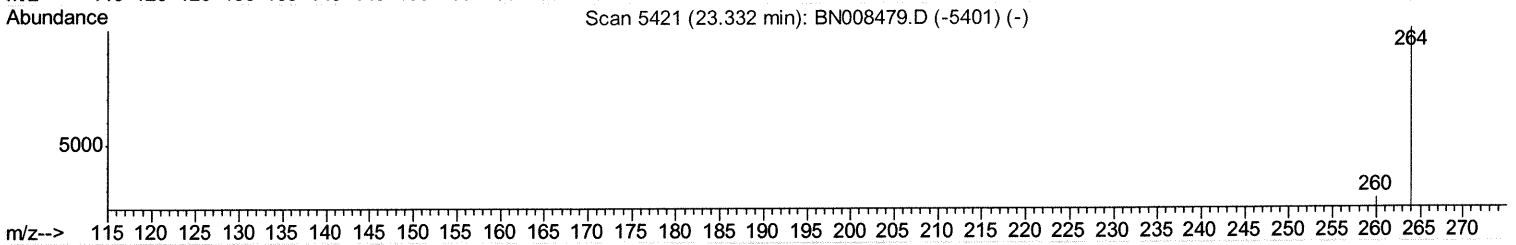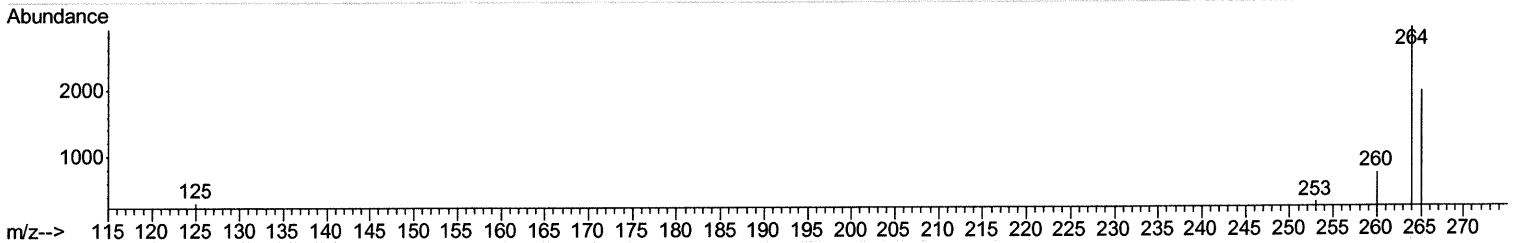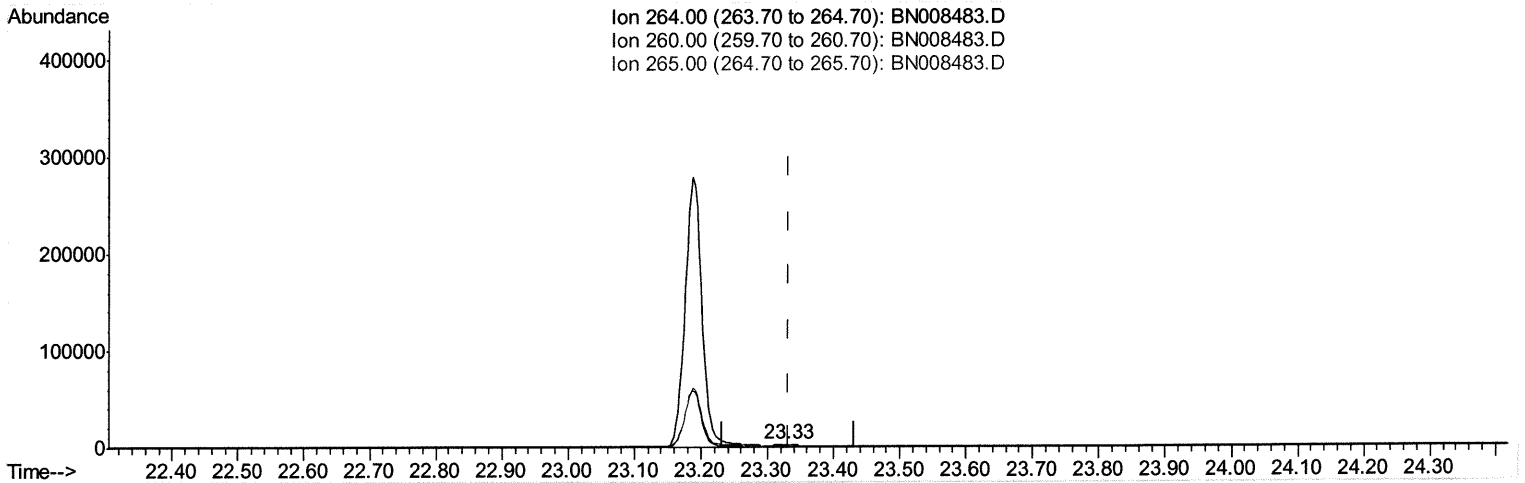

TIC: BN008483.D

(20) Perylene-d12 (I)

23.328min (-0.004) 0.40ng/ul

response 5721

Ion	Exp%	Act%
264.00	100	100
260.00	27.90	25.12
265.00	98.40	67.43#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (Qedit)




Data File : BN008483.D
Acq On : 07 Nov 2019 14:02
Operator : JU
Sample : PB124530BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK30

Manual Integrations
APPROVED

mohammad
11/11/2019 8:07:55 AM

Quant Time: Nov 08 06:00:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration

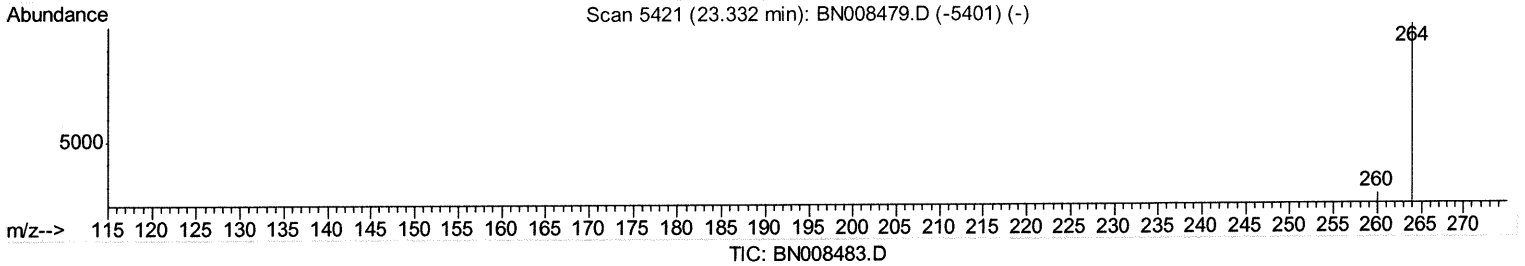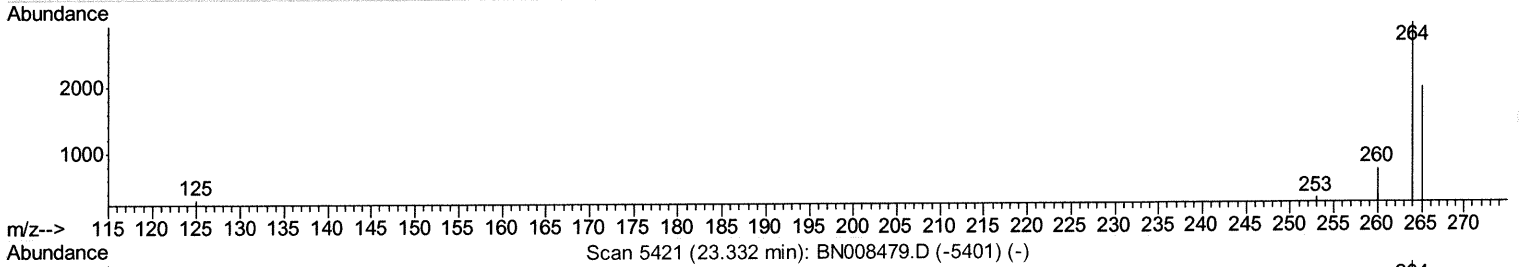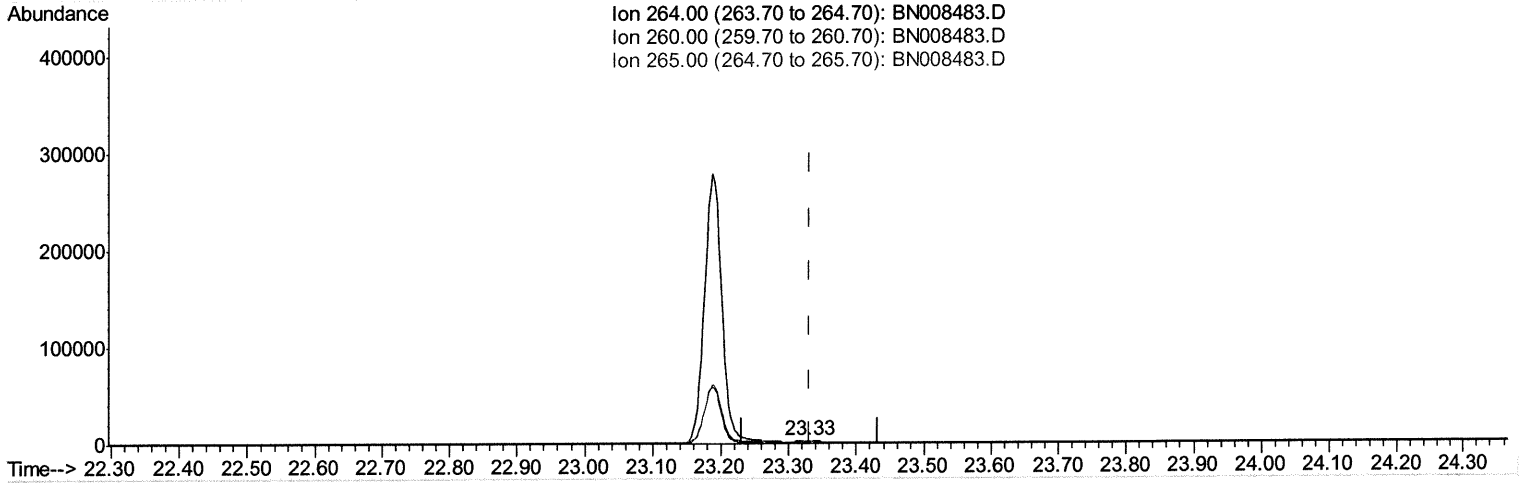

(20) Perylene-d12 (I)

23.328min (-0.004) 0.40ng/ul m

JU 11/11/19

response 2951

Ion	Exp%	Act%
264.00	100	100
260.00	27.90	25.12
265.00	98.40	67.43#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (QT Reviewed)

Data File : BN008483.D
Acq On : 07 Nov 2019 14:02
Operator : JU
Sample : PB124530BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK30

Manual Integrations
APPROVED

mohammad
11/11/2019 8:07:55 AM

Quant Time: Nov 08 06:03:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	1224	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.31	136	4820	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.19	164	2445	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.94	188	4518m	0.40	ng/ul	0.00
16) Chrysene-d12	21.16	240	3554	0.40	ng/ul	0.00
20) Perylene-d12	23.33	264	2951m	0.40	ng/ul	0.00

Ju 11/11/19
Ju 11/11/19

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.93	152	2531	0.33	ng/ul	0.00
14) Fluoranthene-d10	18.99	212	5416	0.40	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed